

This Page Is Inserted by IFW Operations
and is not a part of the Official Record

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

IMAGES ARE BEST AVAILABLE COPY.

**As rescanning documents *will not* correct images,
please do not report the images to the
Image Problem Mailbox.**

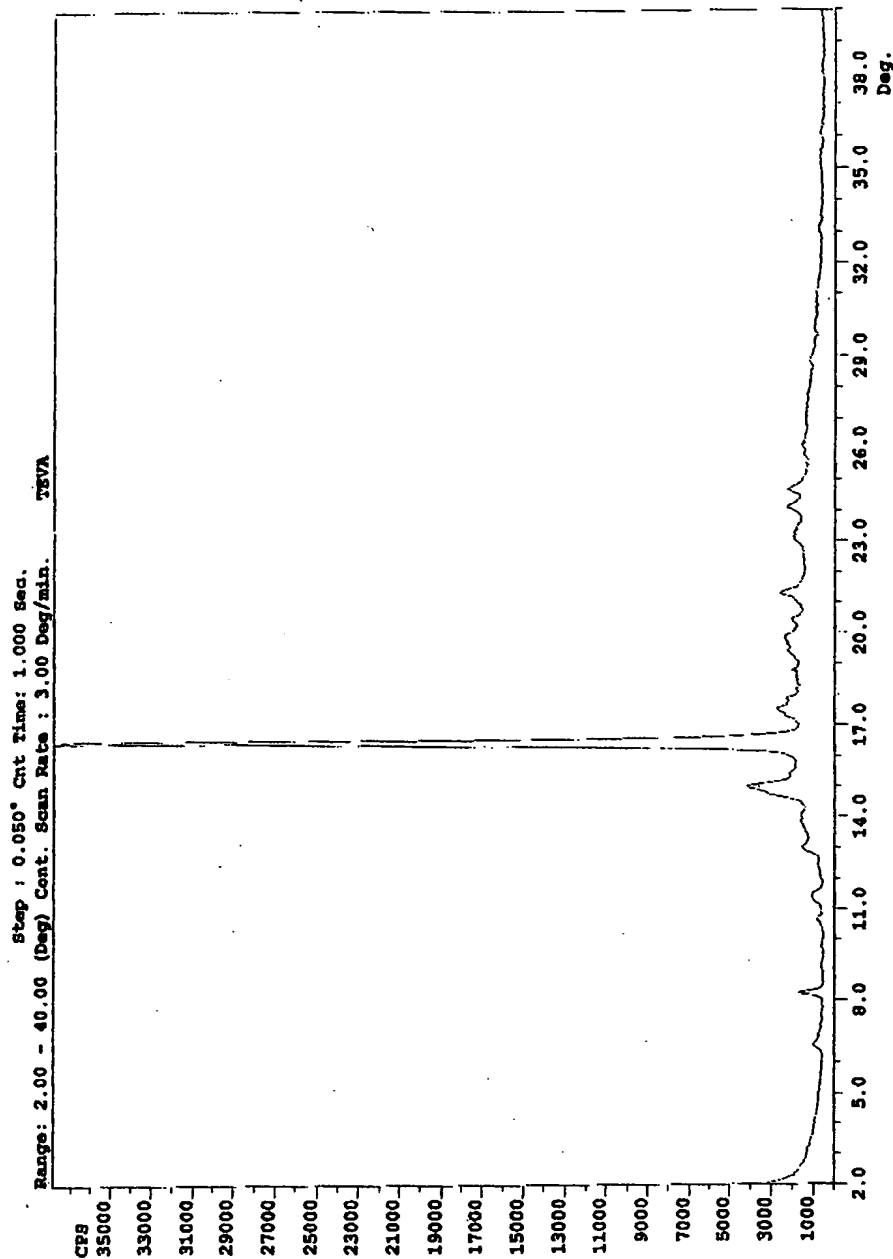


Figure 1

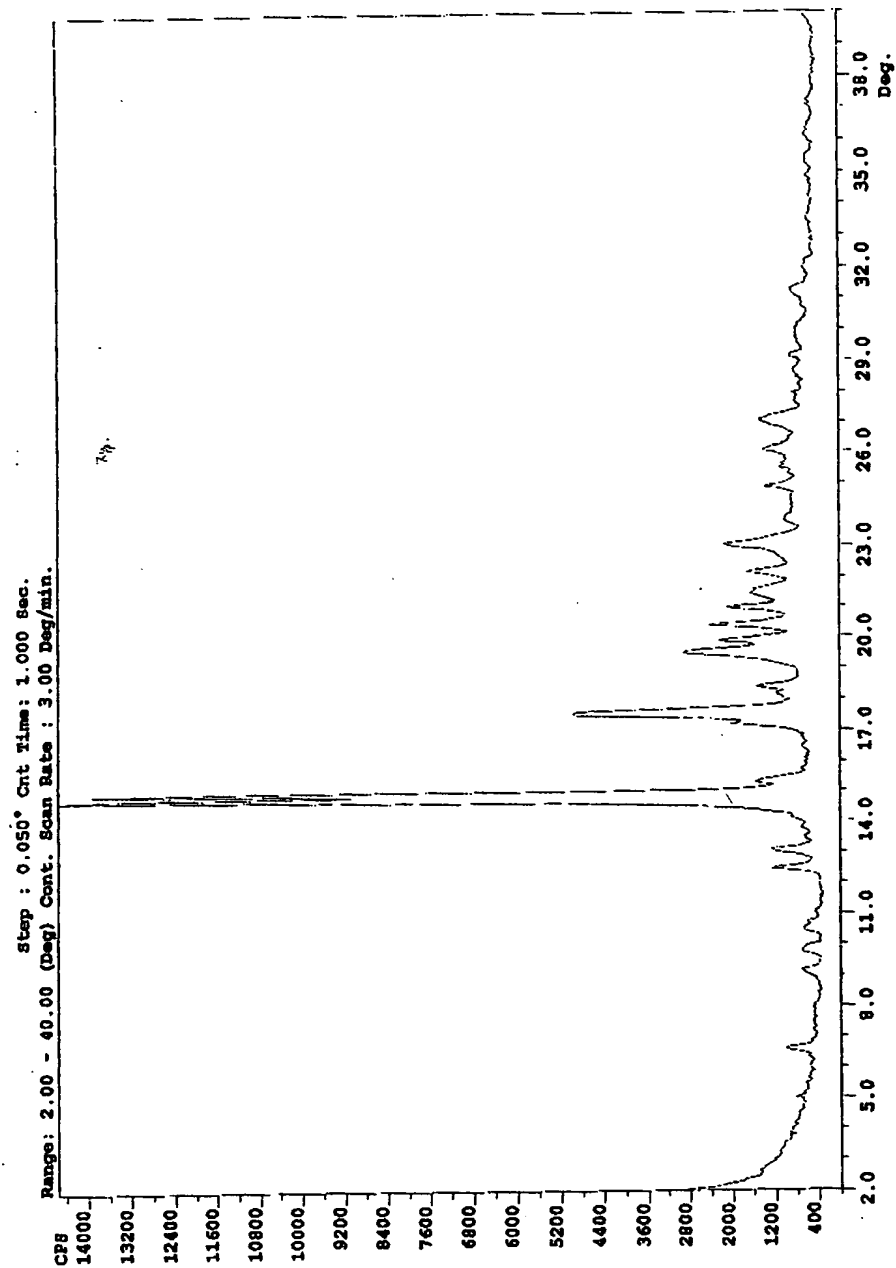


Figure 2

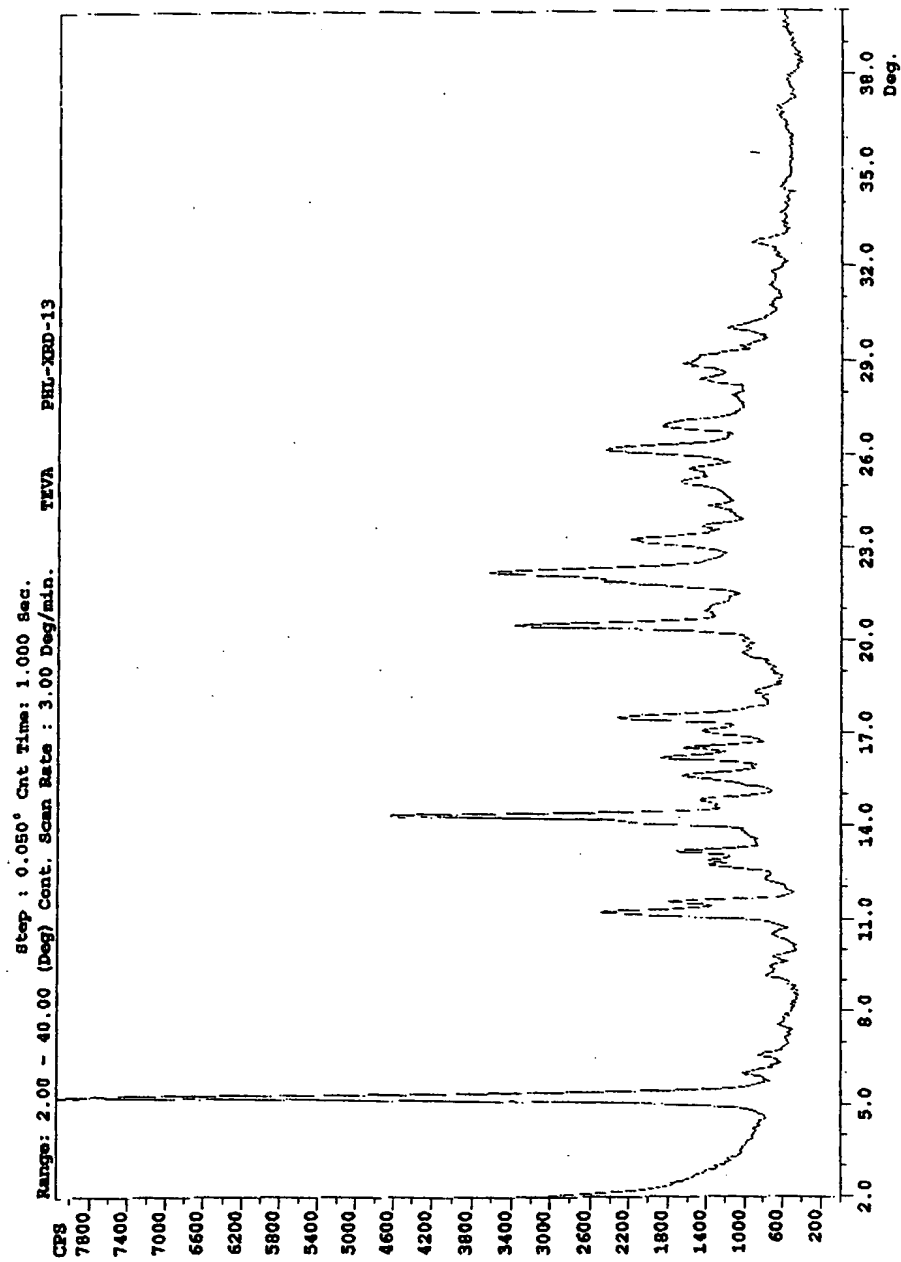


Figure 3

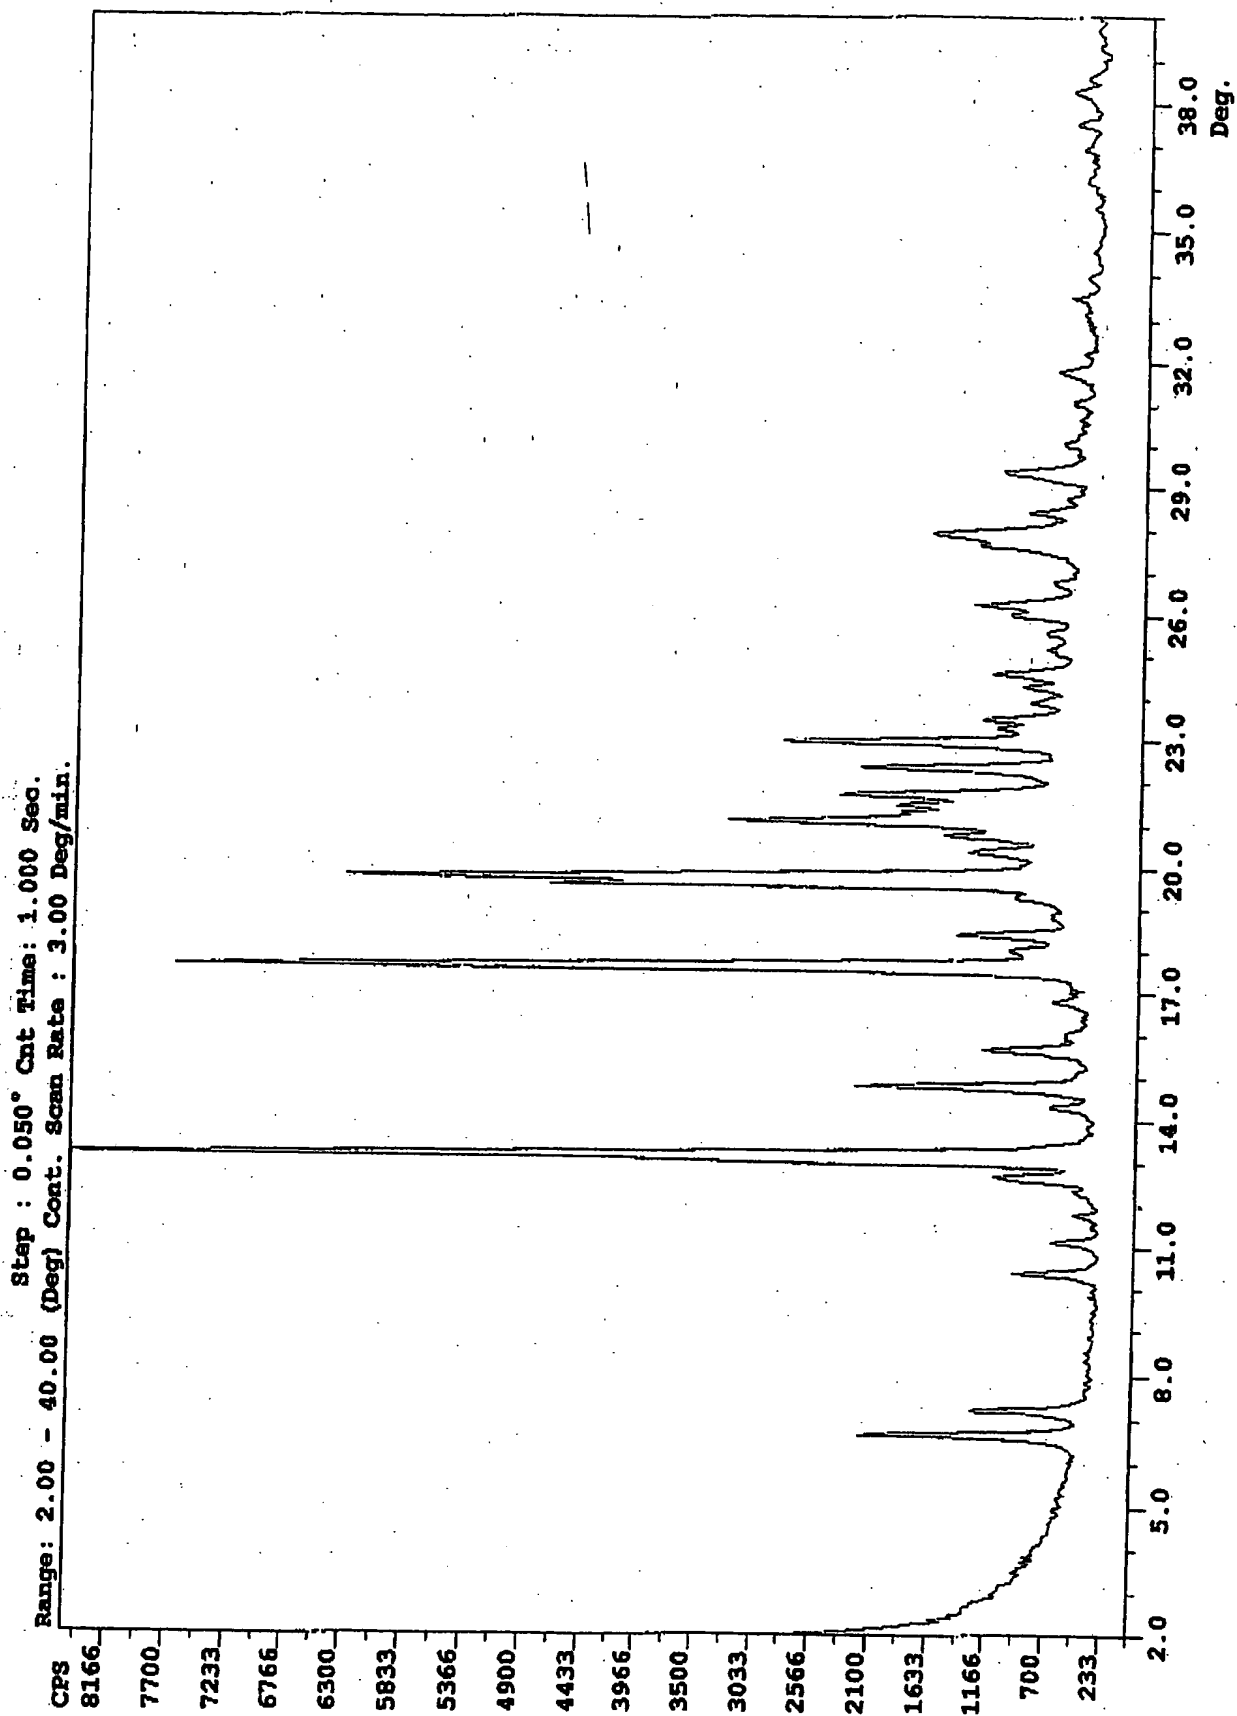


Figure 4

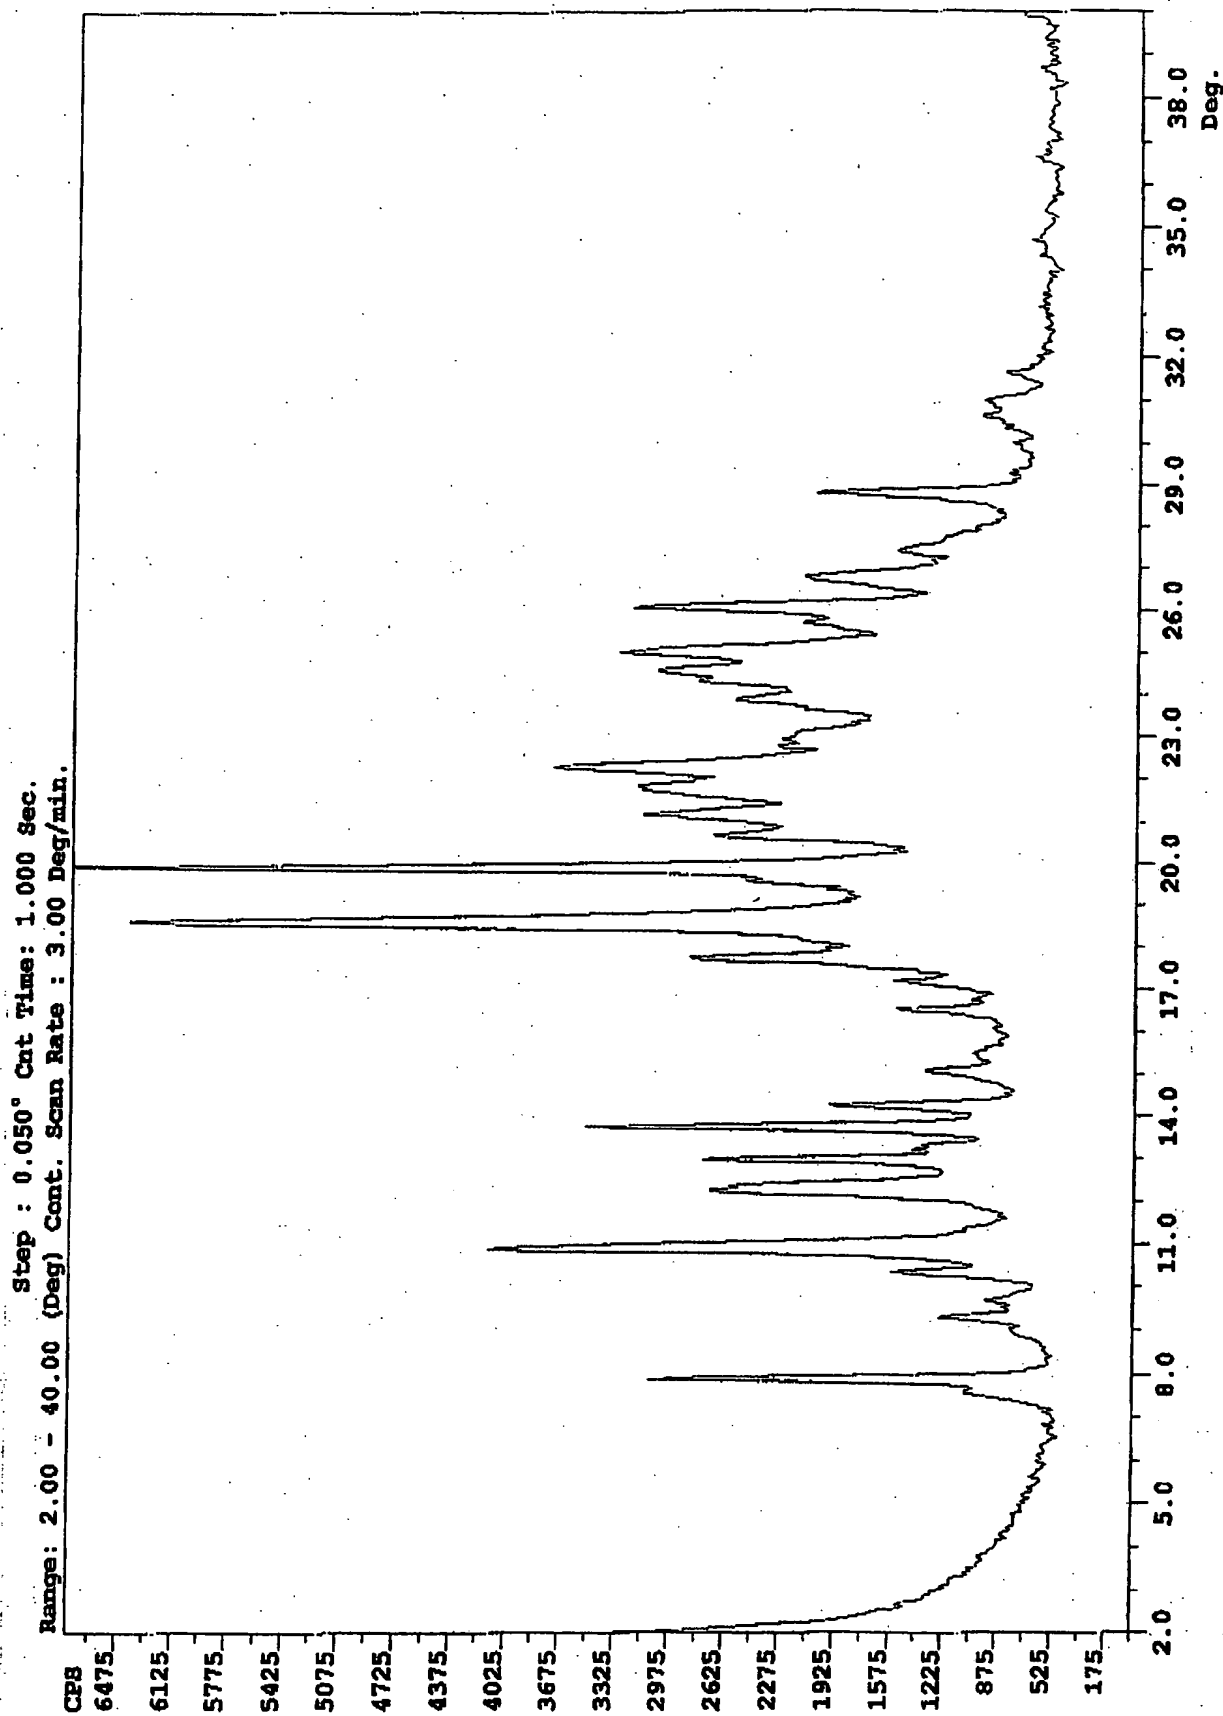


Figure 5

Step : 0.050° Cnt Time: 1.000 Sec.
Range: 2.00 - 40.00 (Deg) Cnt. Scan Rate : 3.00 Deg/min.

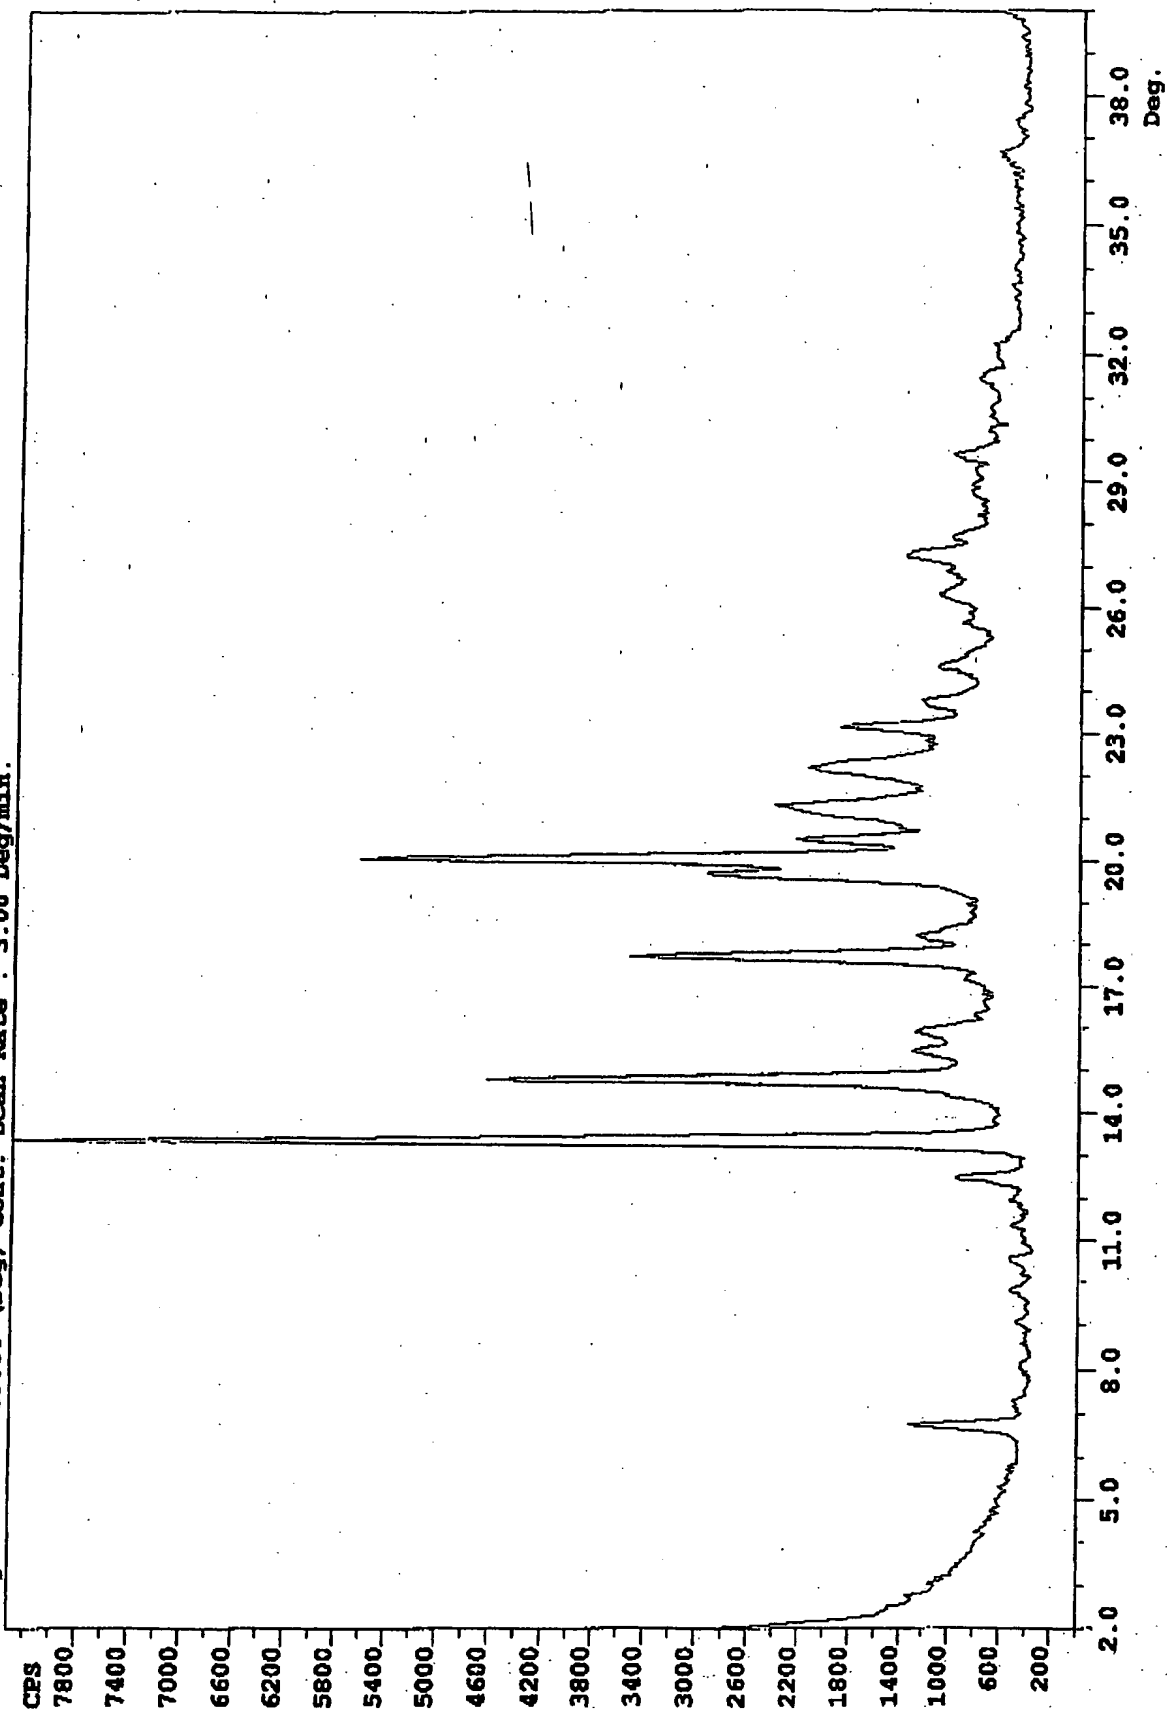


Figure 6

Step : 0.050° Cnt Time: 1.000 Sec.
Range: 2.00 - 40.00 (Deg) Cnt. Scan Rate : 3.00 Deg/min.

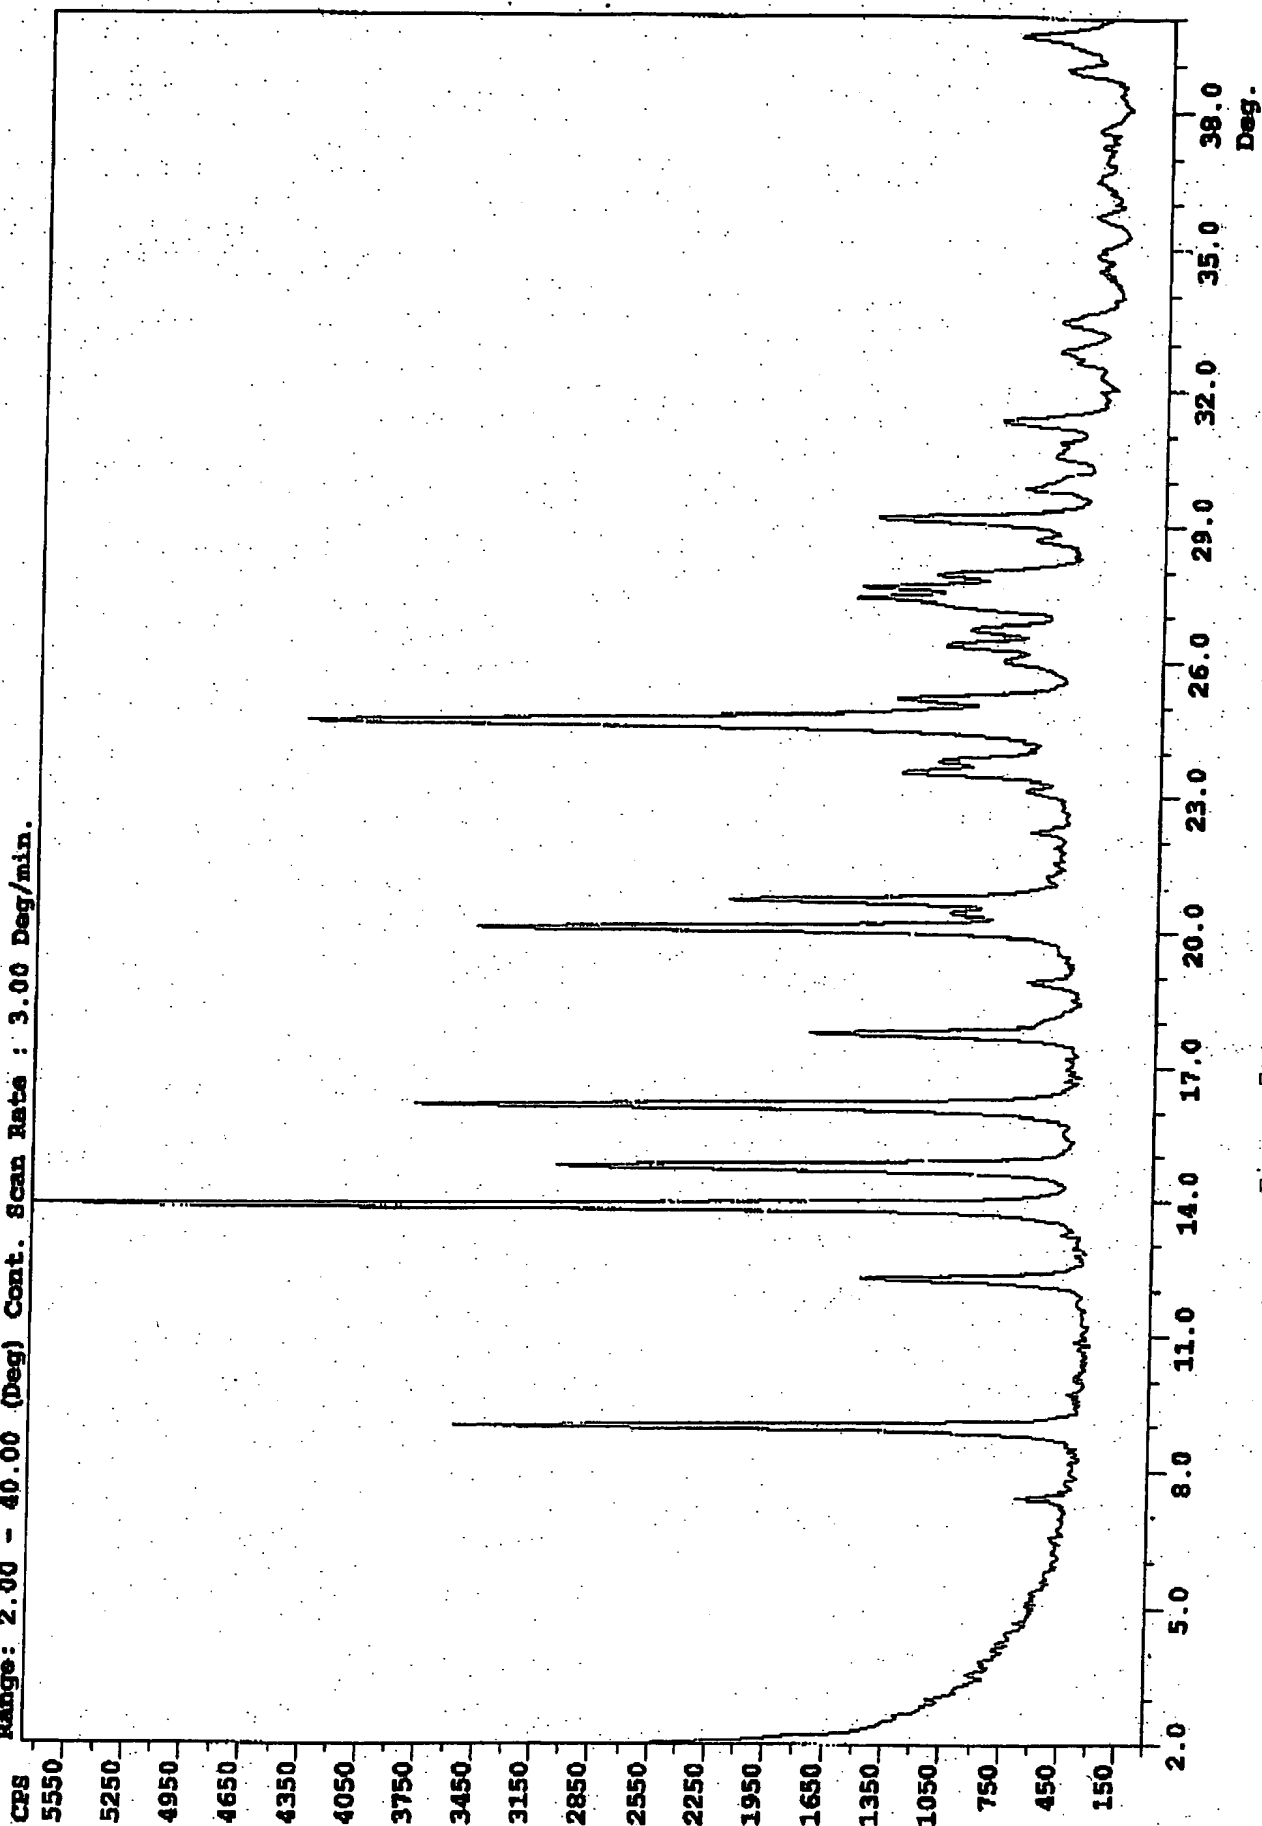


Figure 7

Step : 0.050° Cnt Time: 1.000 Sec.
Range: 2.00 - 40.00 (Deg) Cnt. Scan Rate : 3.00 Deg/min.

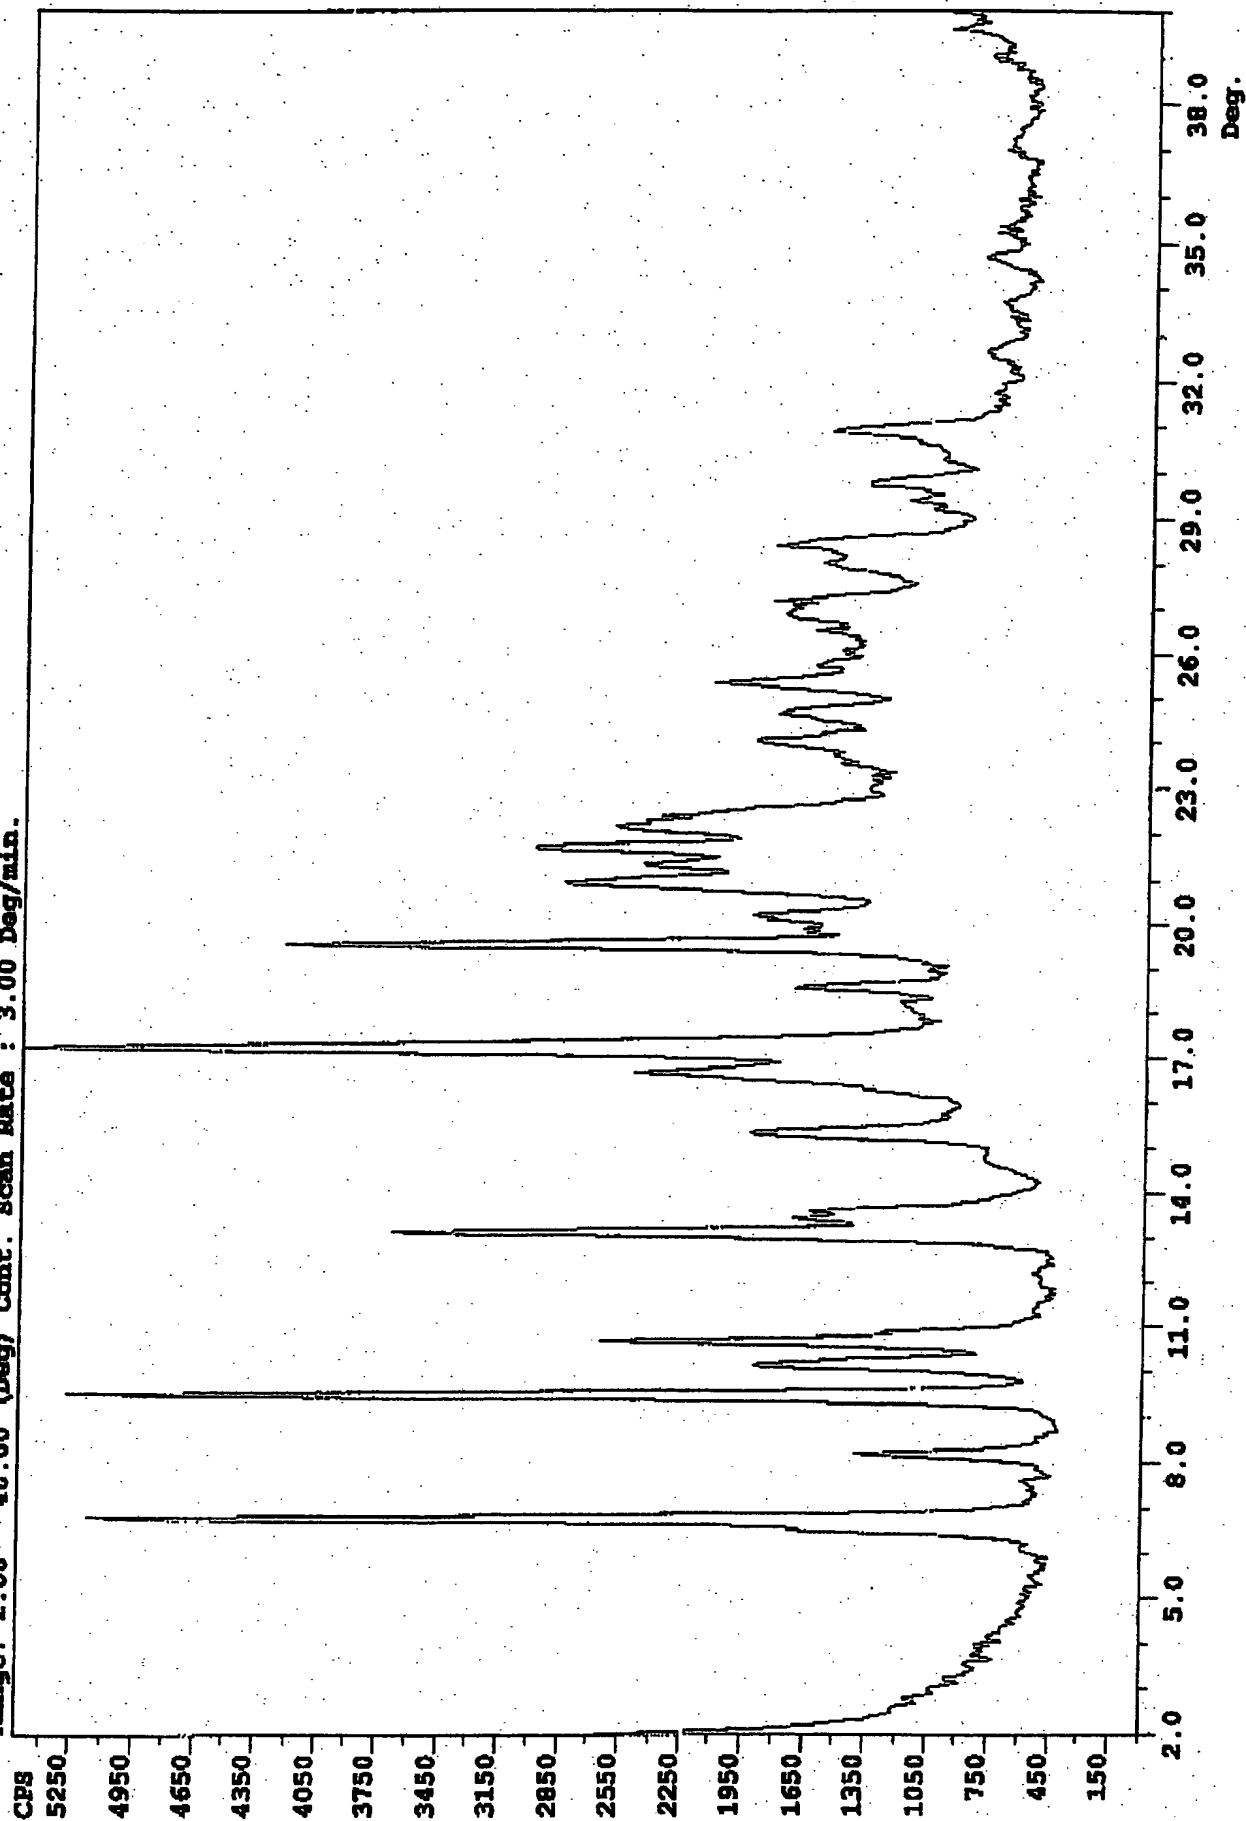


Figure 8

Step : 0.050° Cnt Time: 1.000 Sec.
Range: 2.00 - 40.00 (Deg) Cnt. Scan Rate : 3.00 Deg/min.

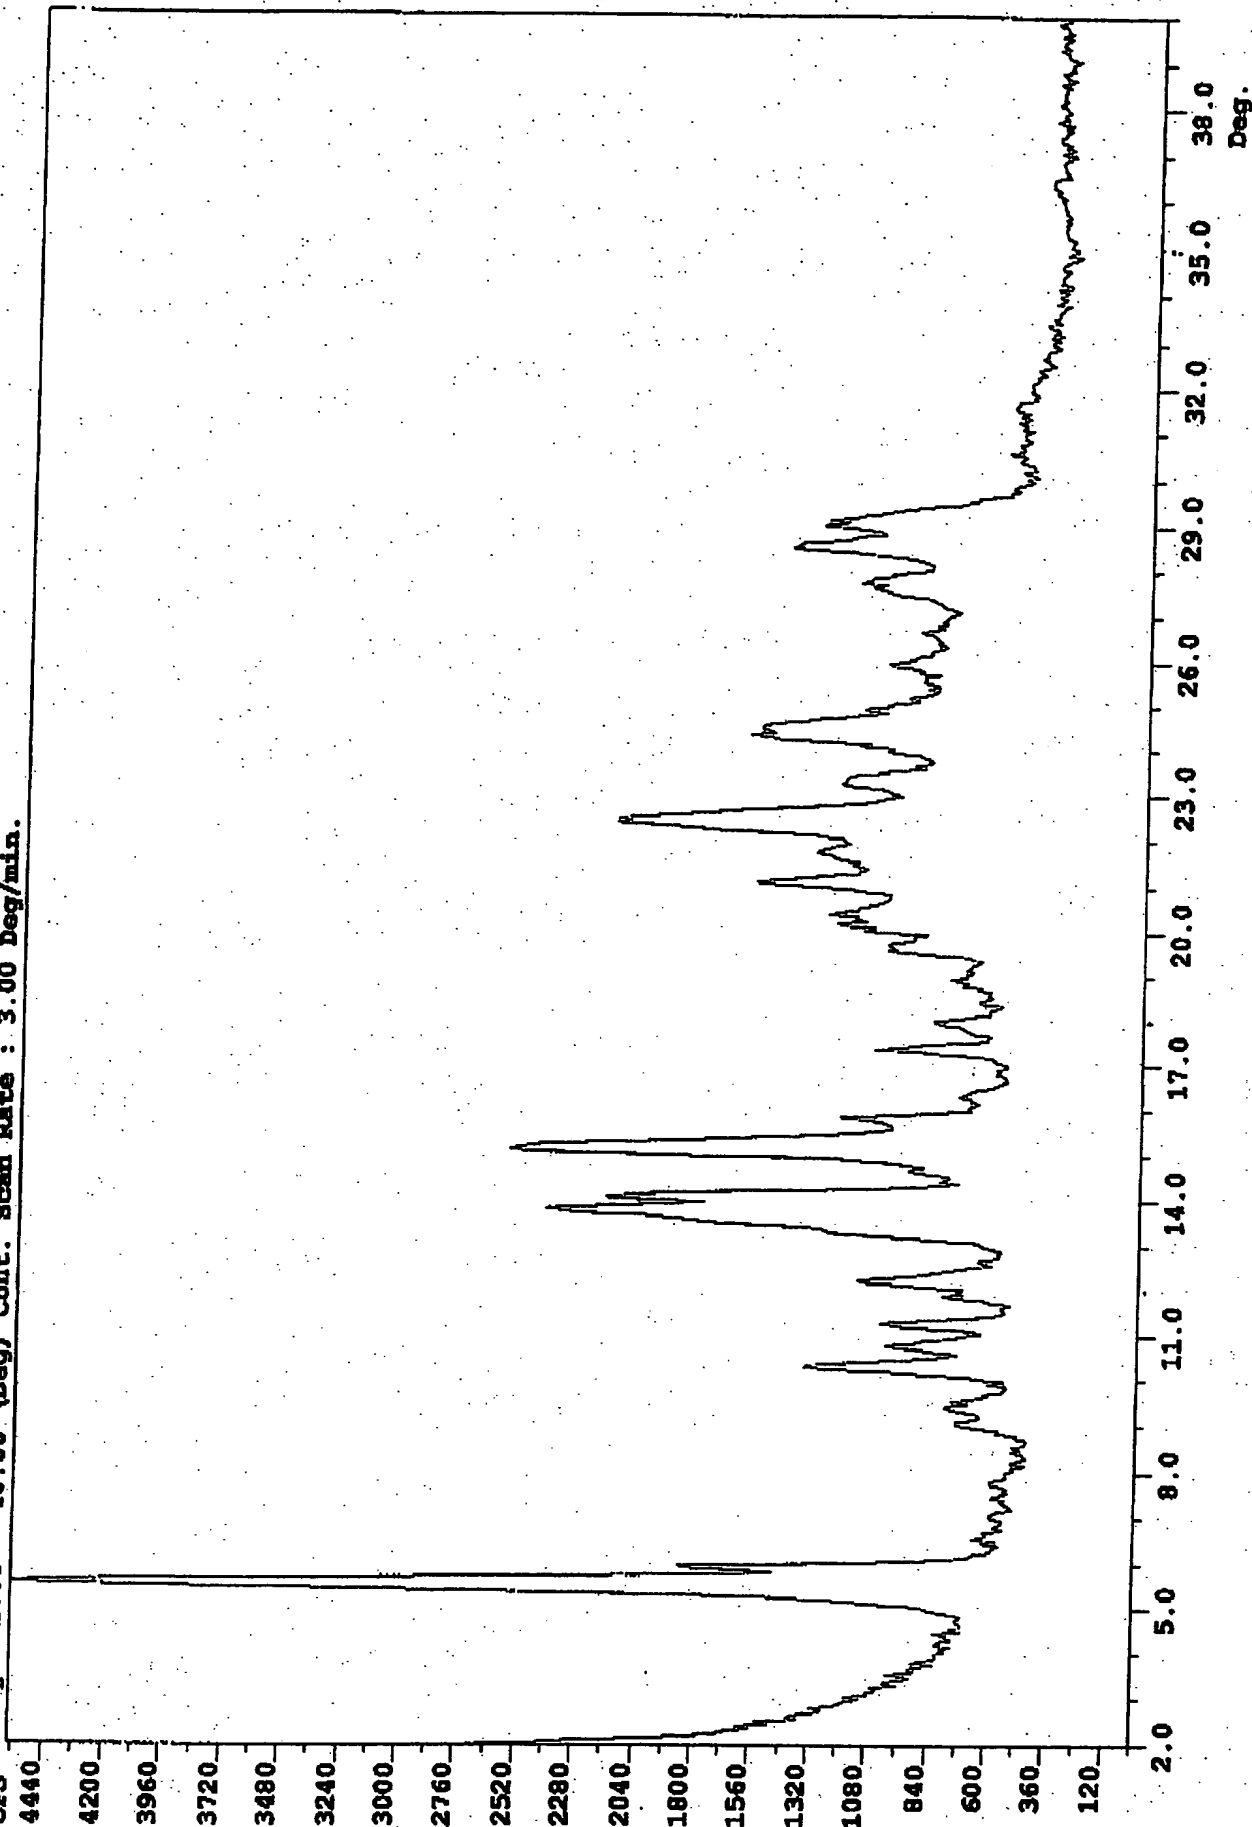


Figure 9

Step : 0.050° Cnt Time: 1.000 Sec.
Range: 2.00 - 40.00 (Deg) Cnt. Scan Rate : 3.00 Deg/min.

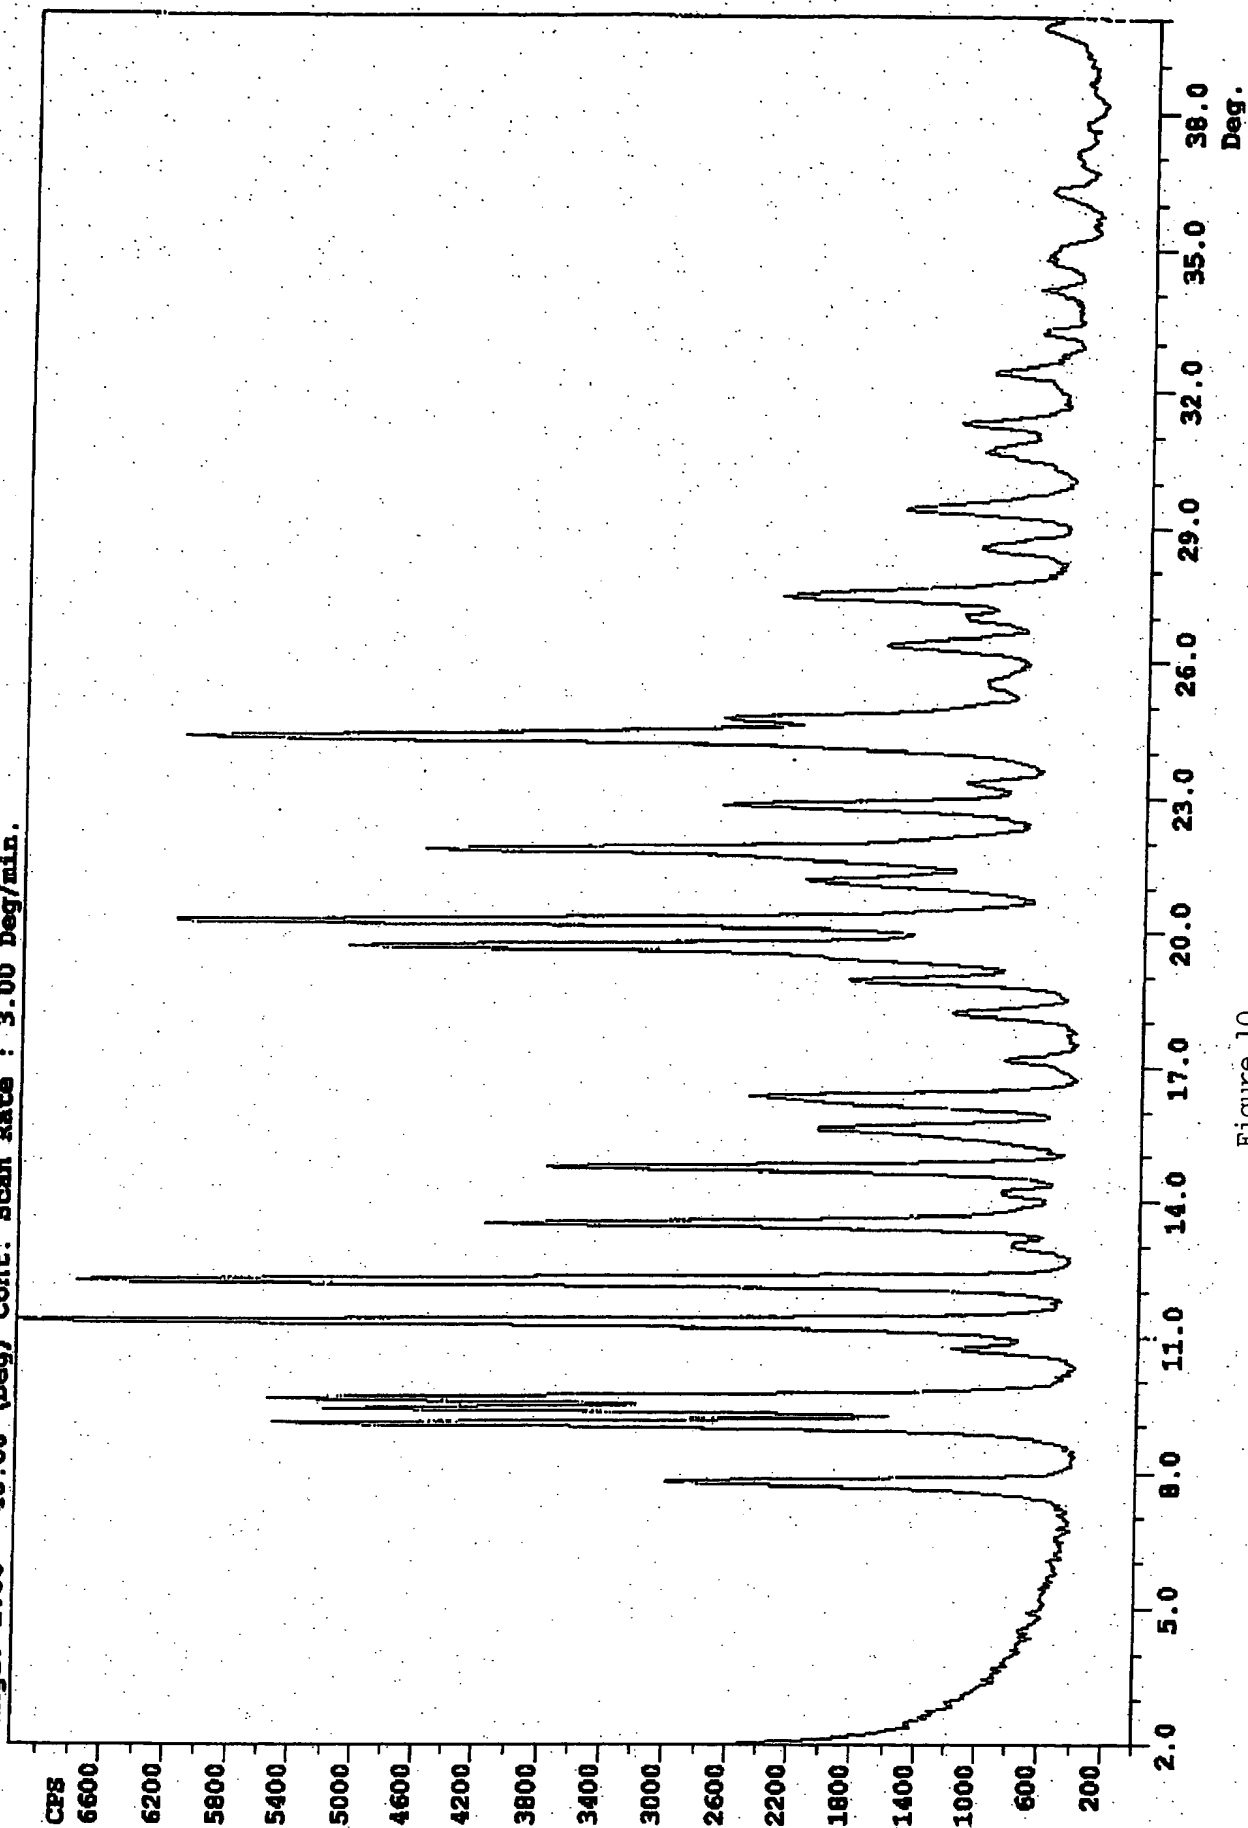


Figure 10

Step : 0.050° Cnt Time: 1.000 Sec.
Range: 2.00 - 40.00 (Deg) Cont. Scan Rate : 3.00 Deg/min.

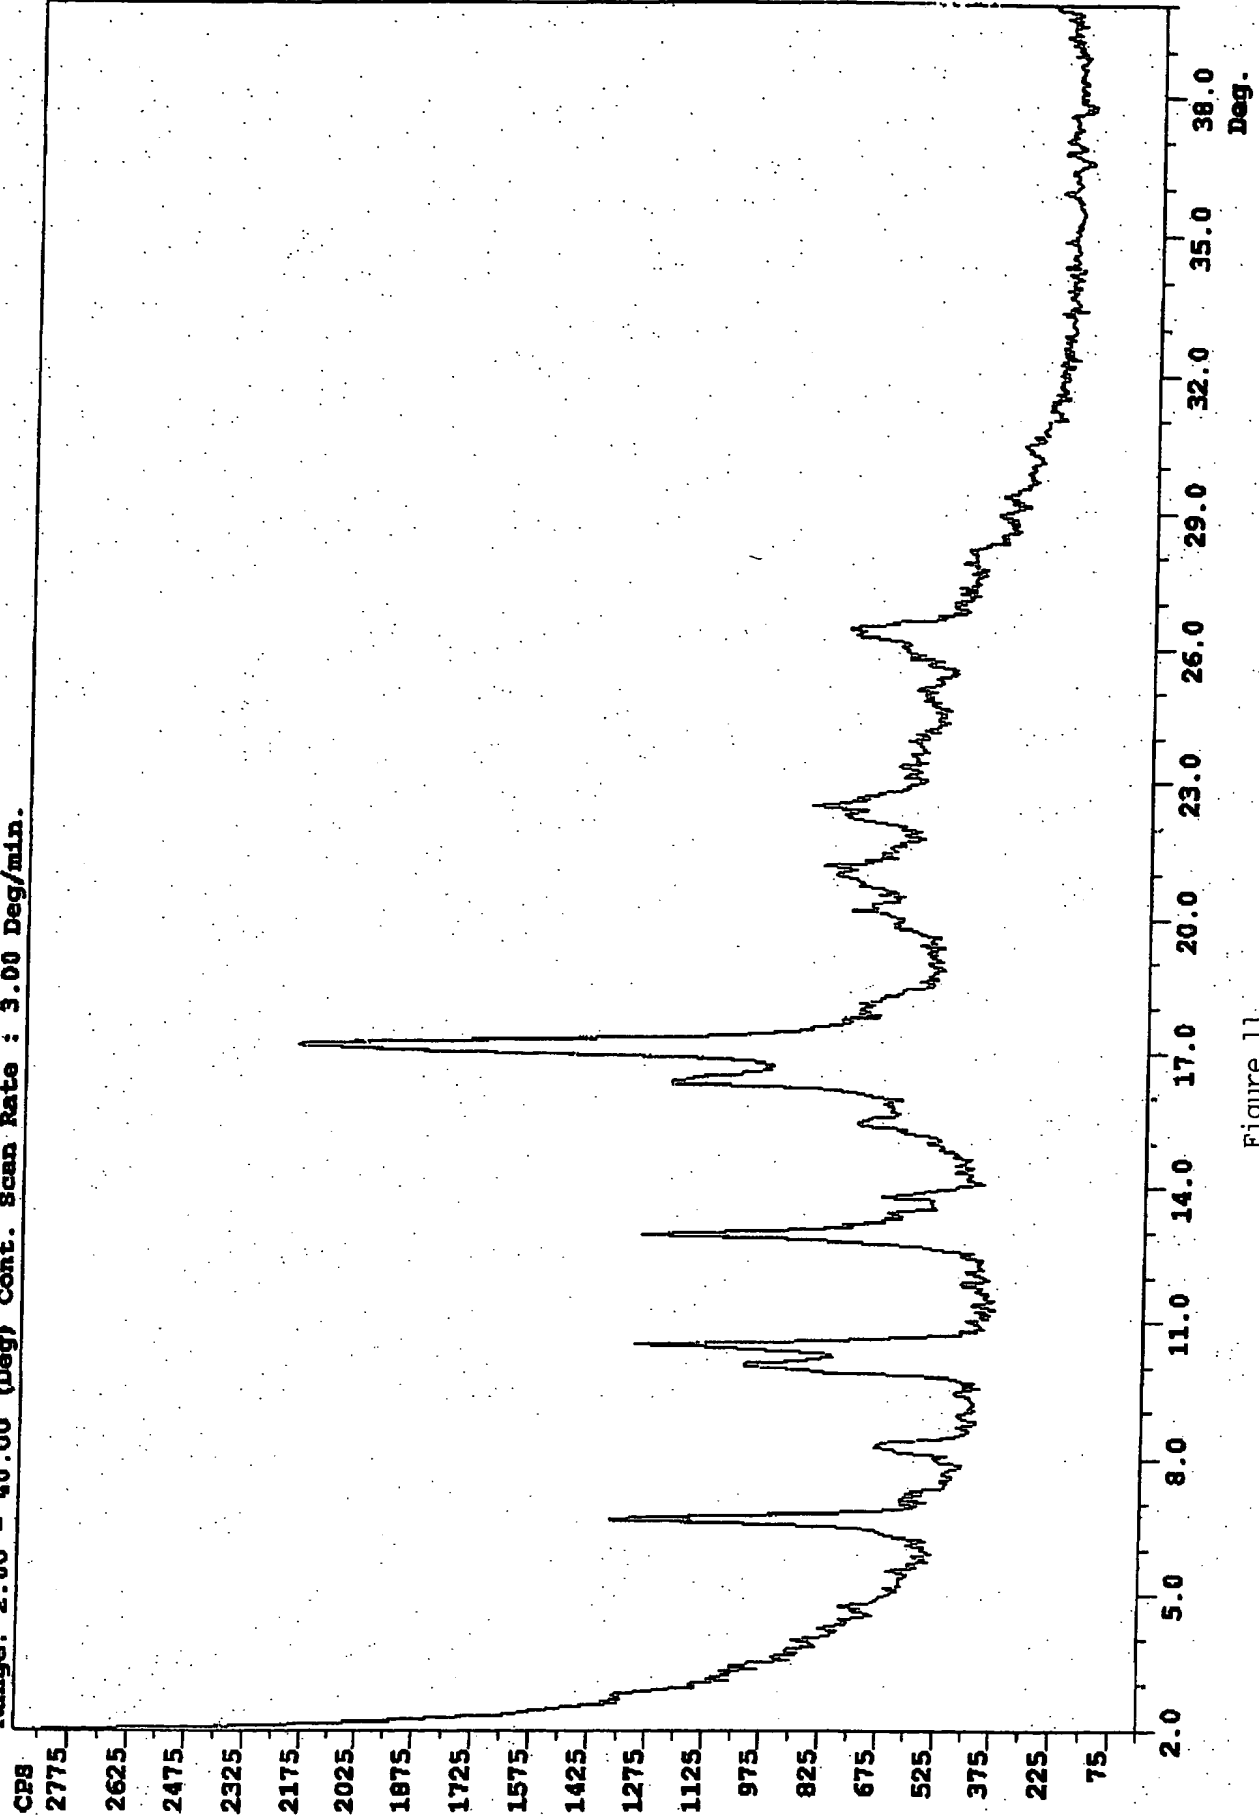


Figure 11

Step : 0.050° Cnt Time: 0.600 Sec.
Range: 5.00 - 30.00 (Deg) Cnt. Scan Rate : 5.00 Deg/min.

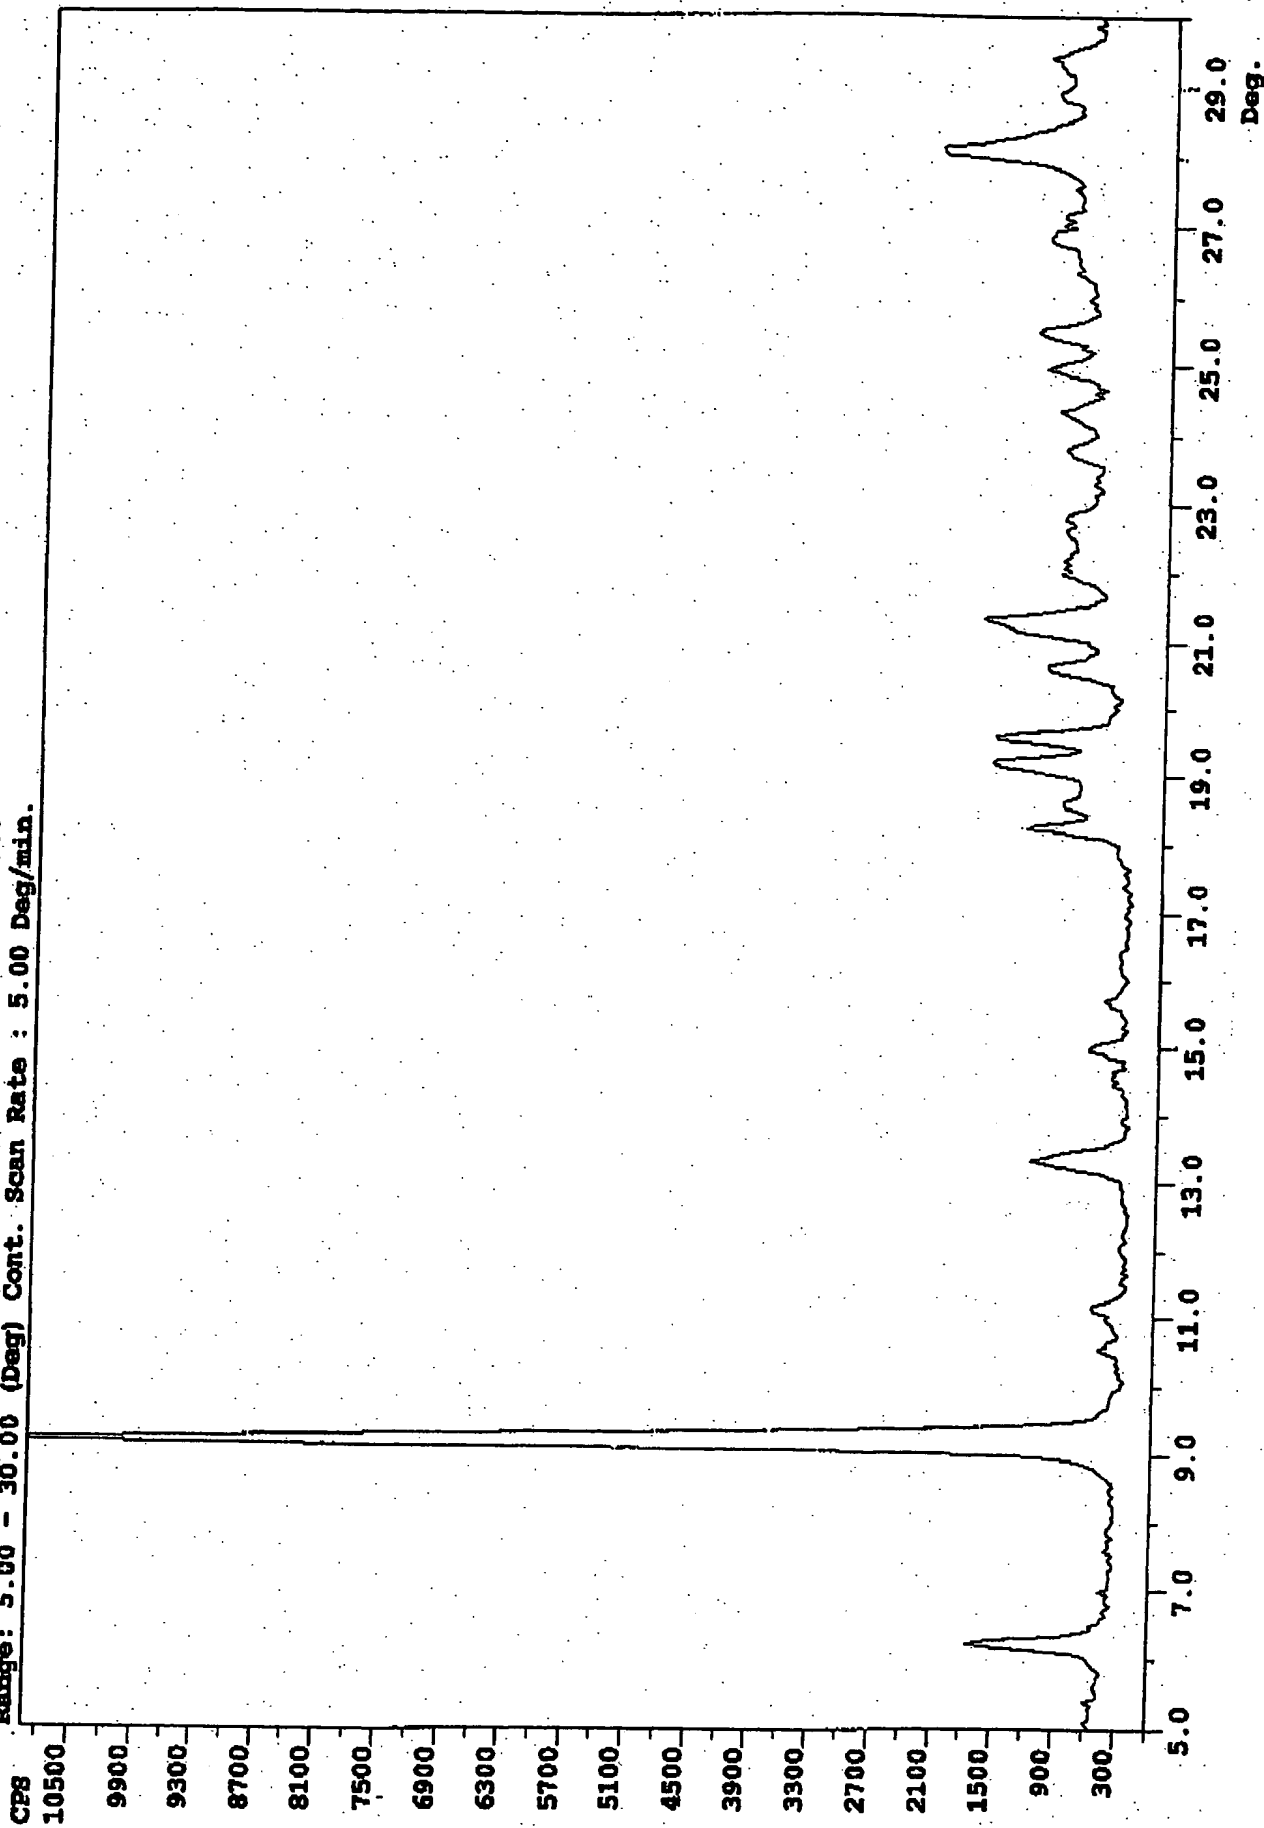


Figure 12

Step : 0.050° Cnt Time: 0.600 Sec.
Range: 5.00 - 30.00 (Deg) Cnt. Scan Rate : 5.00 Deg/min.

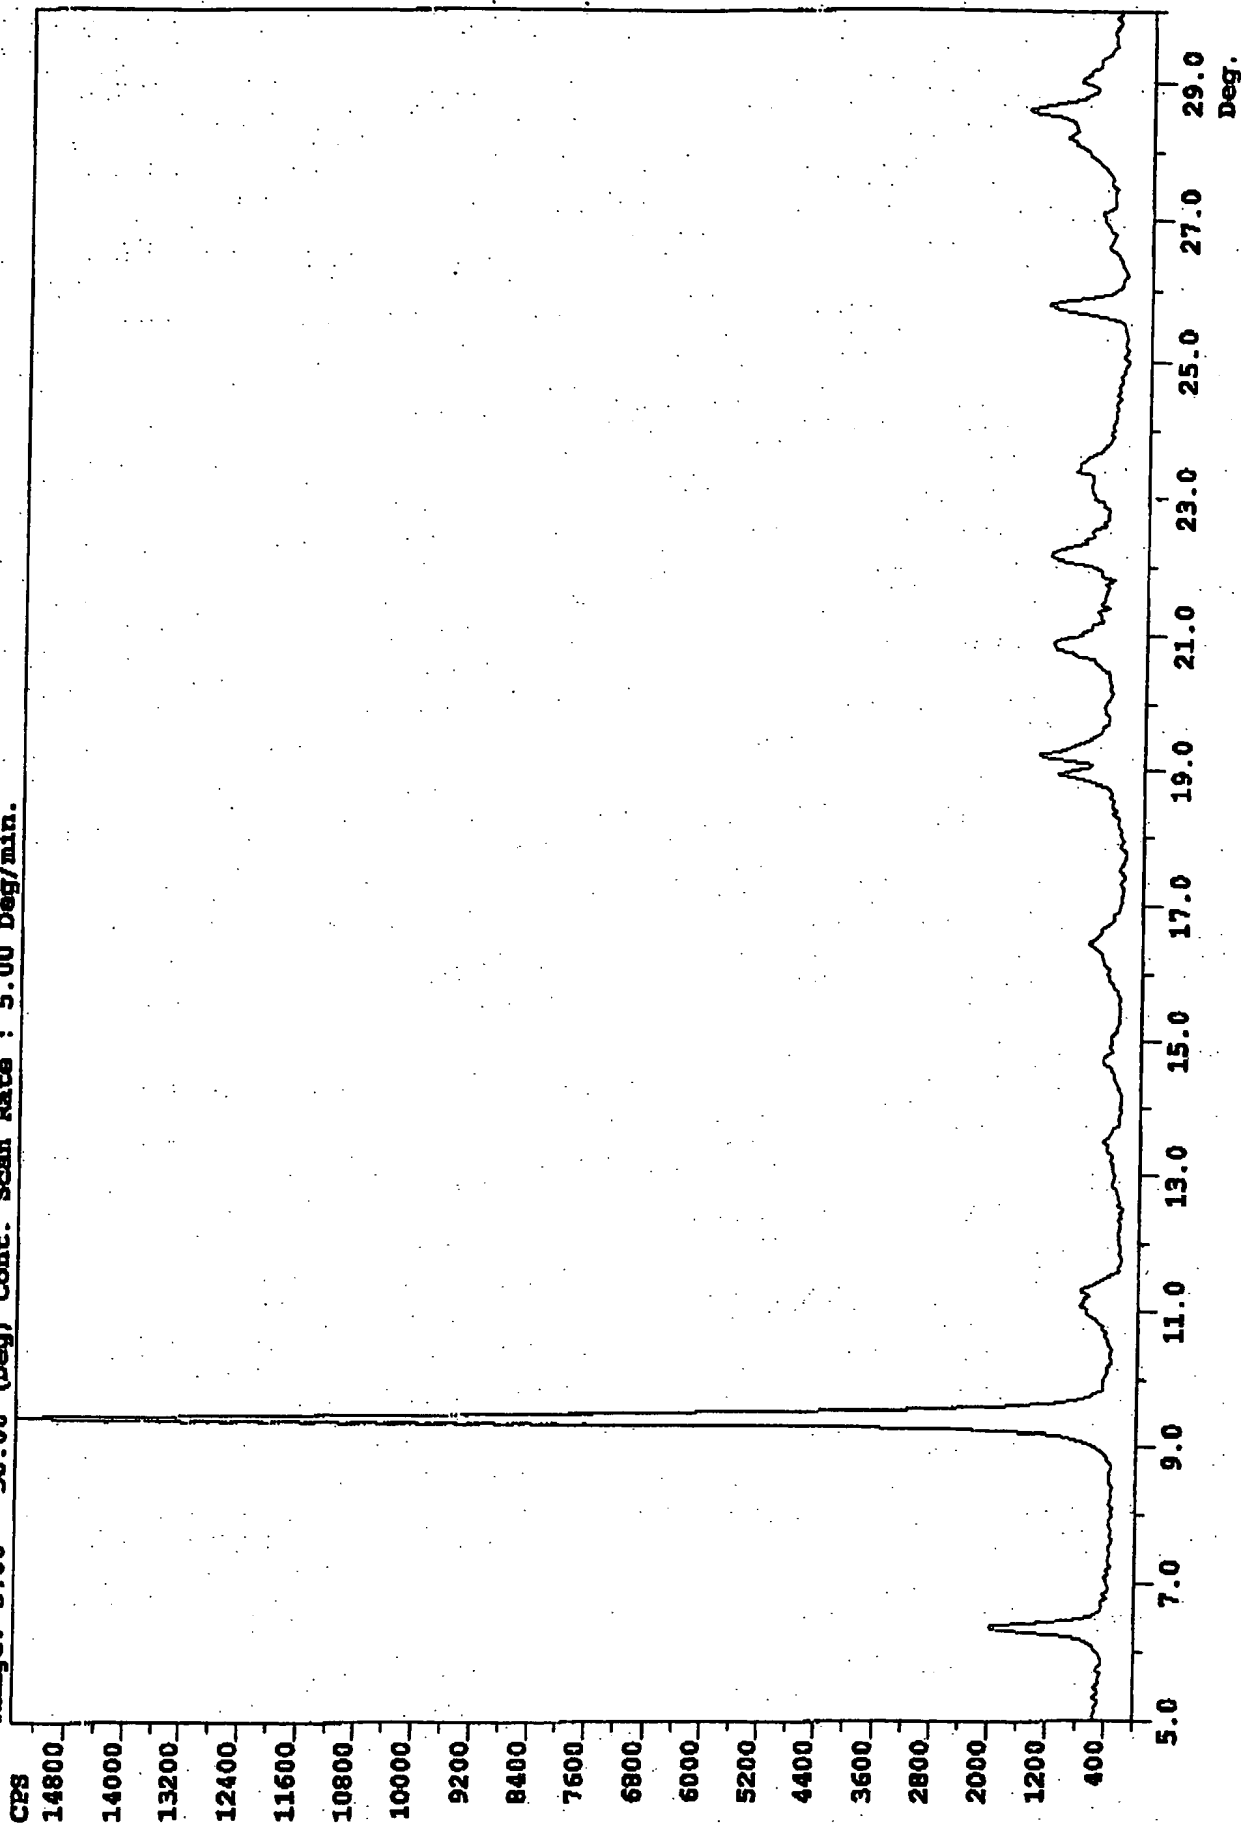


Figure 13

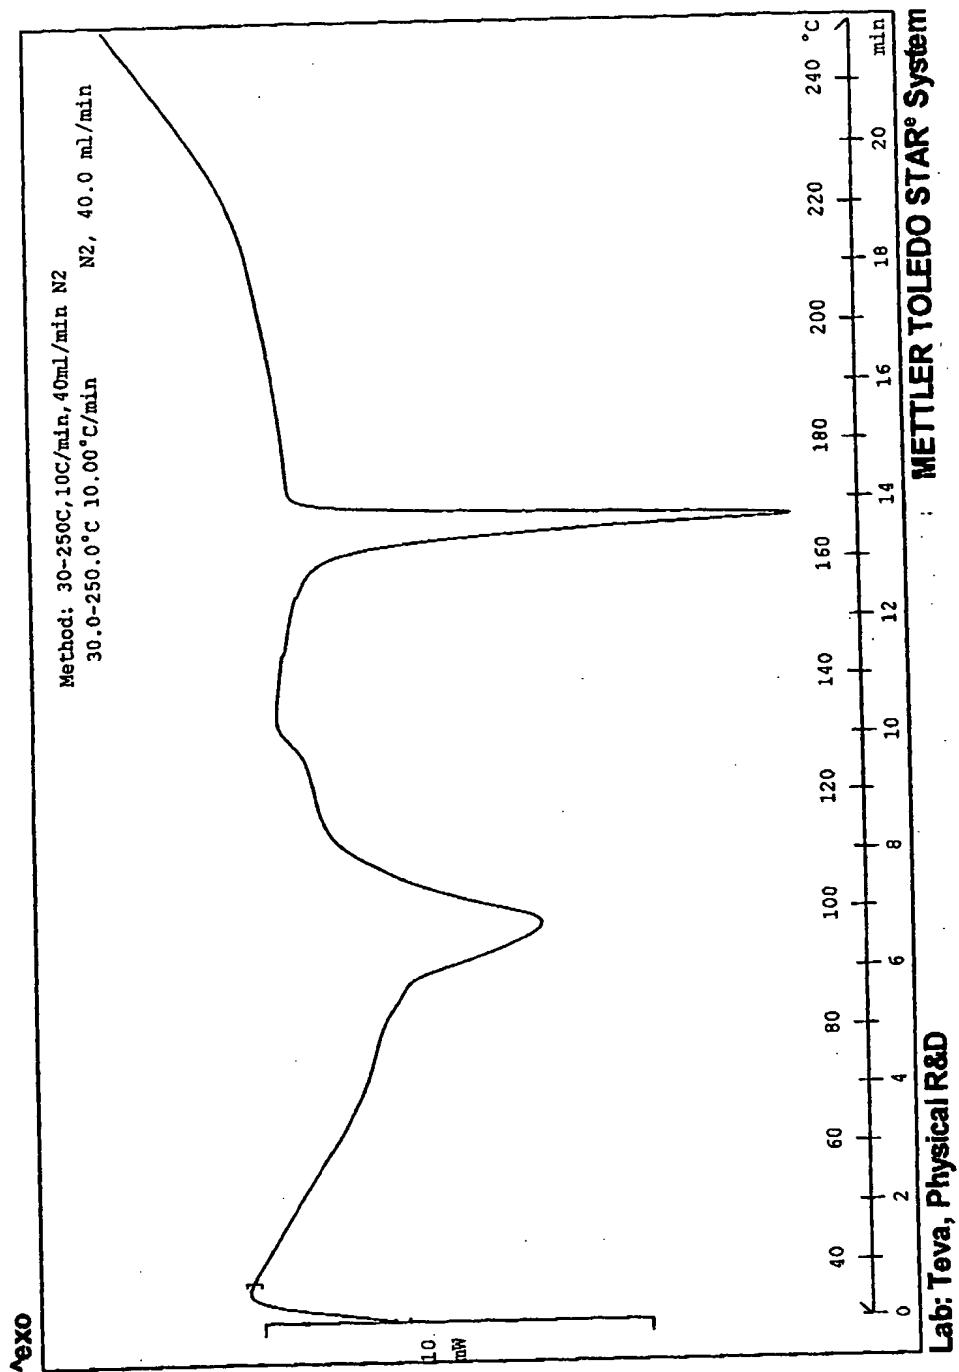


Figure 14

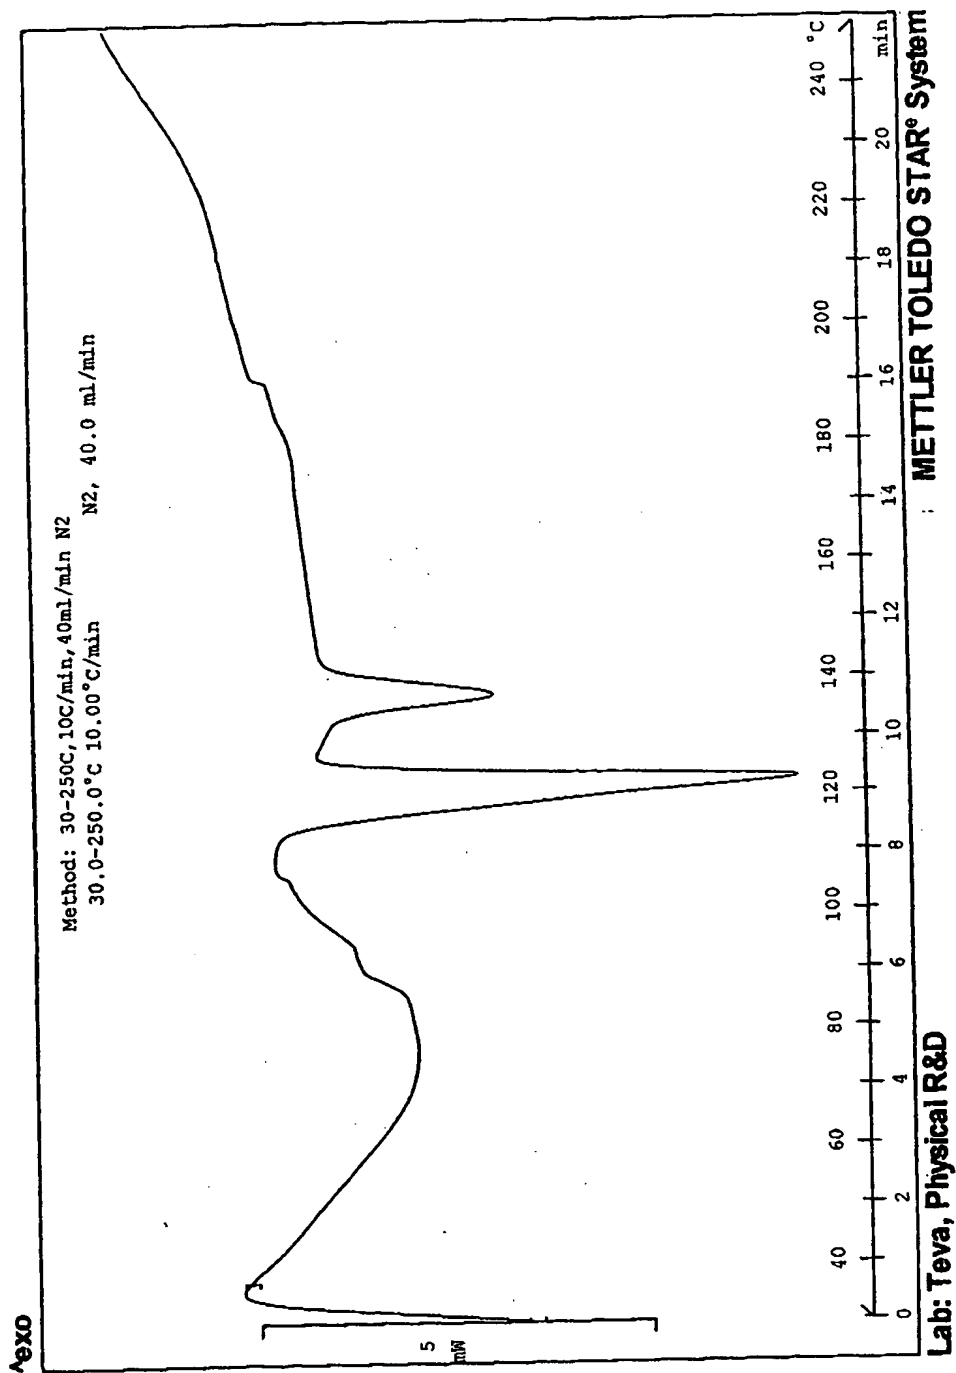


Figure 15

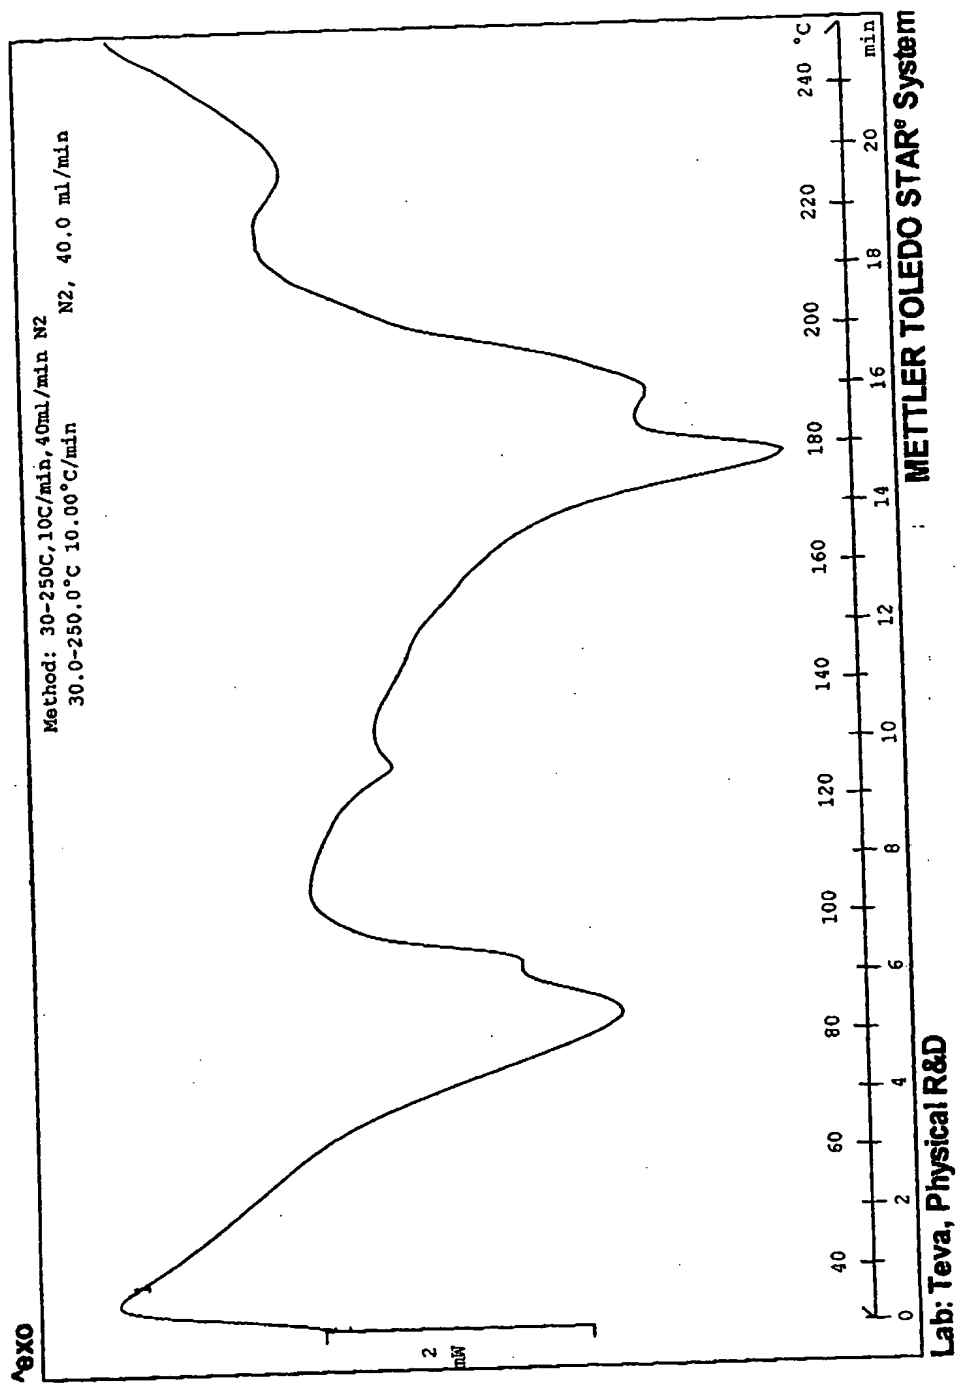


Figure 16

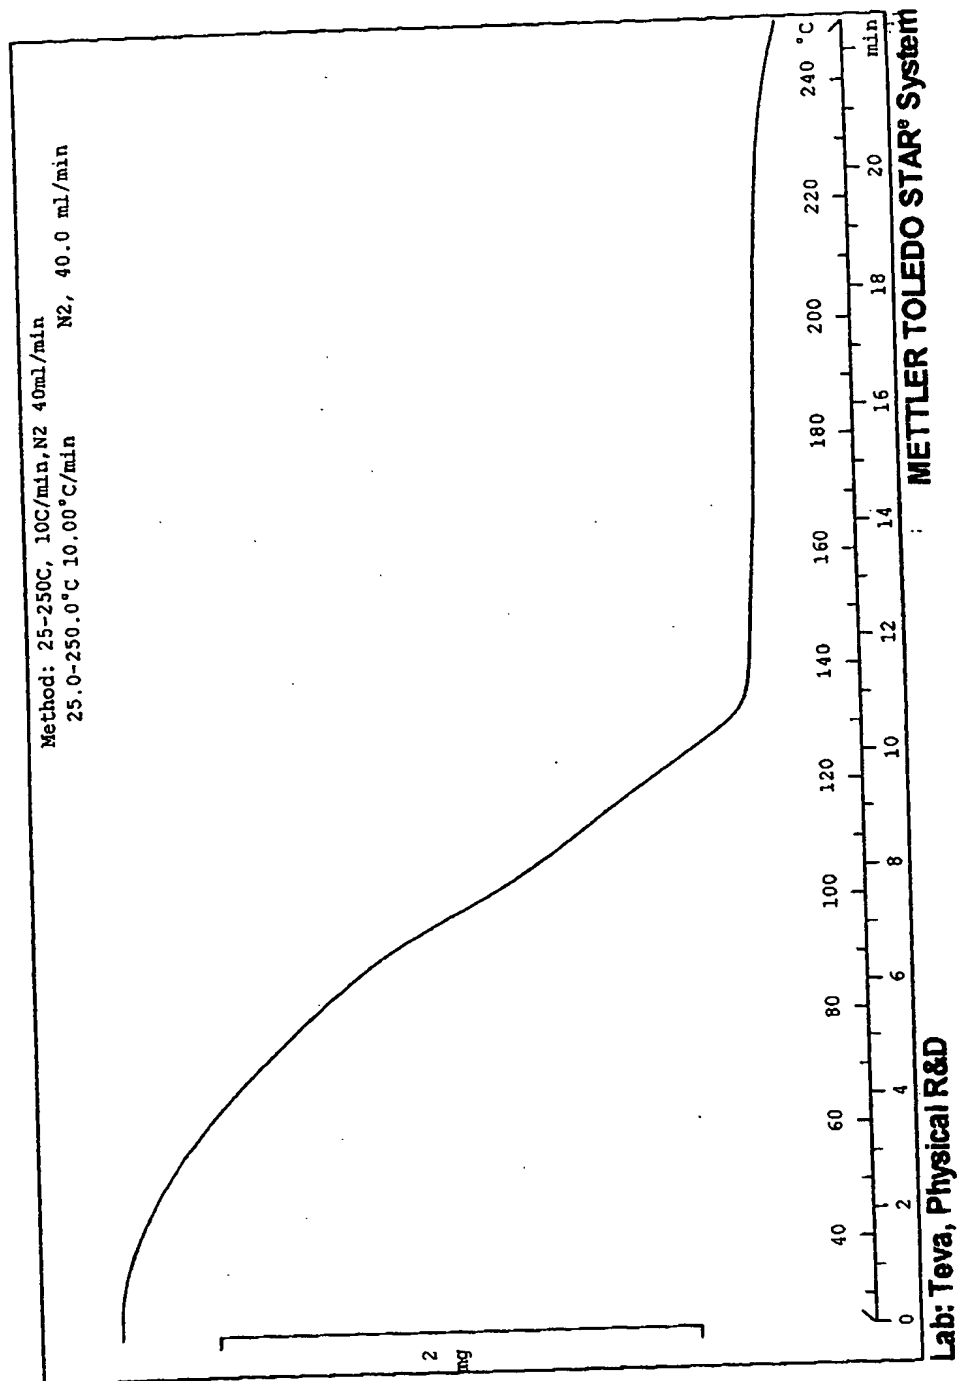


Figure 17

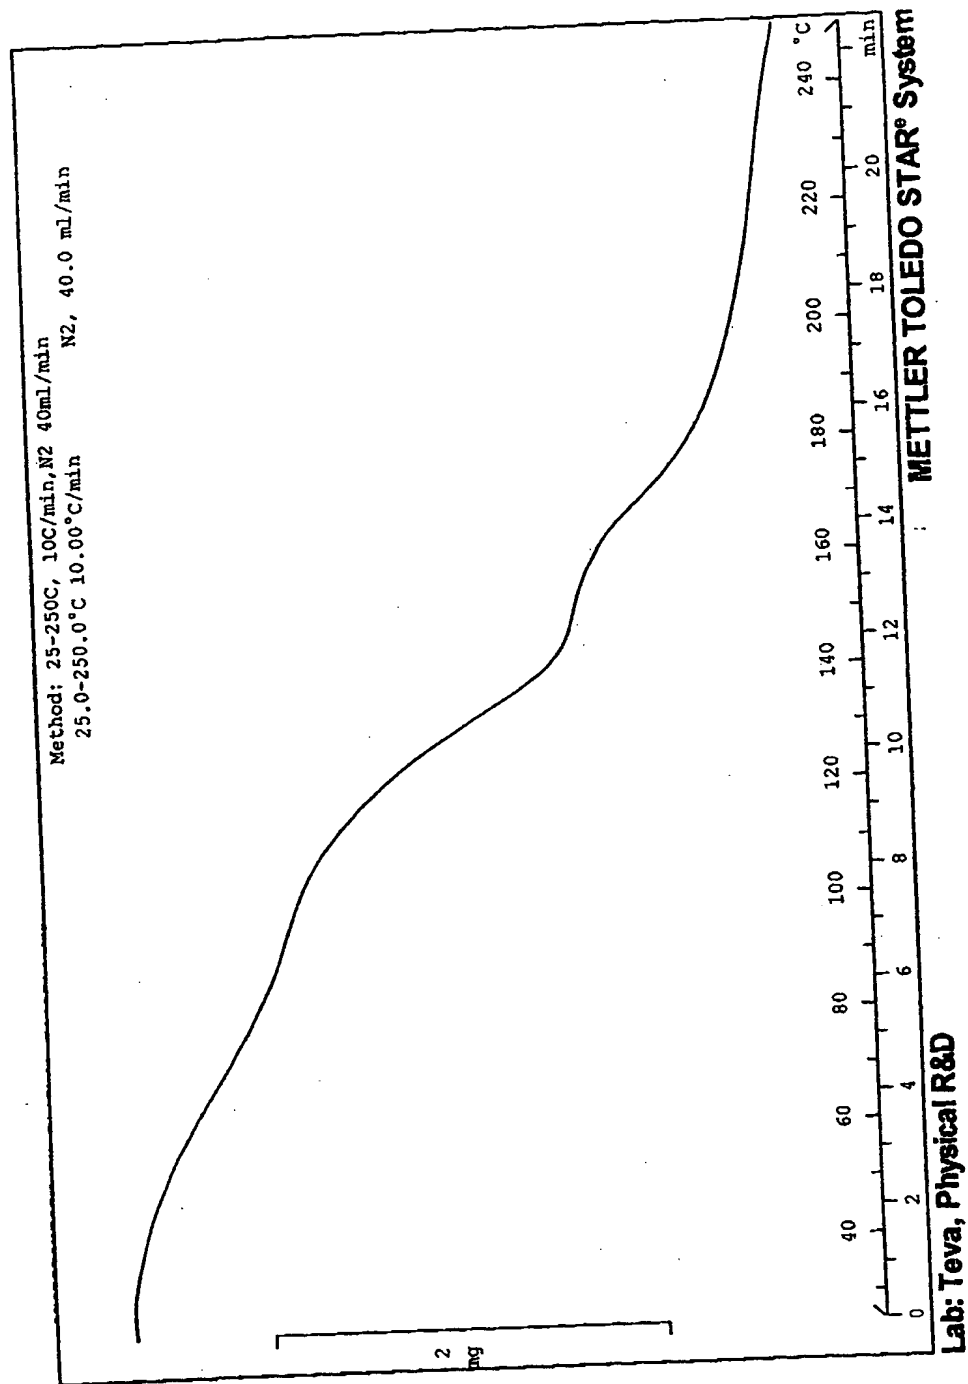


Figure 18


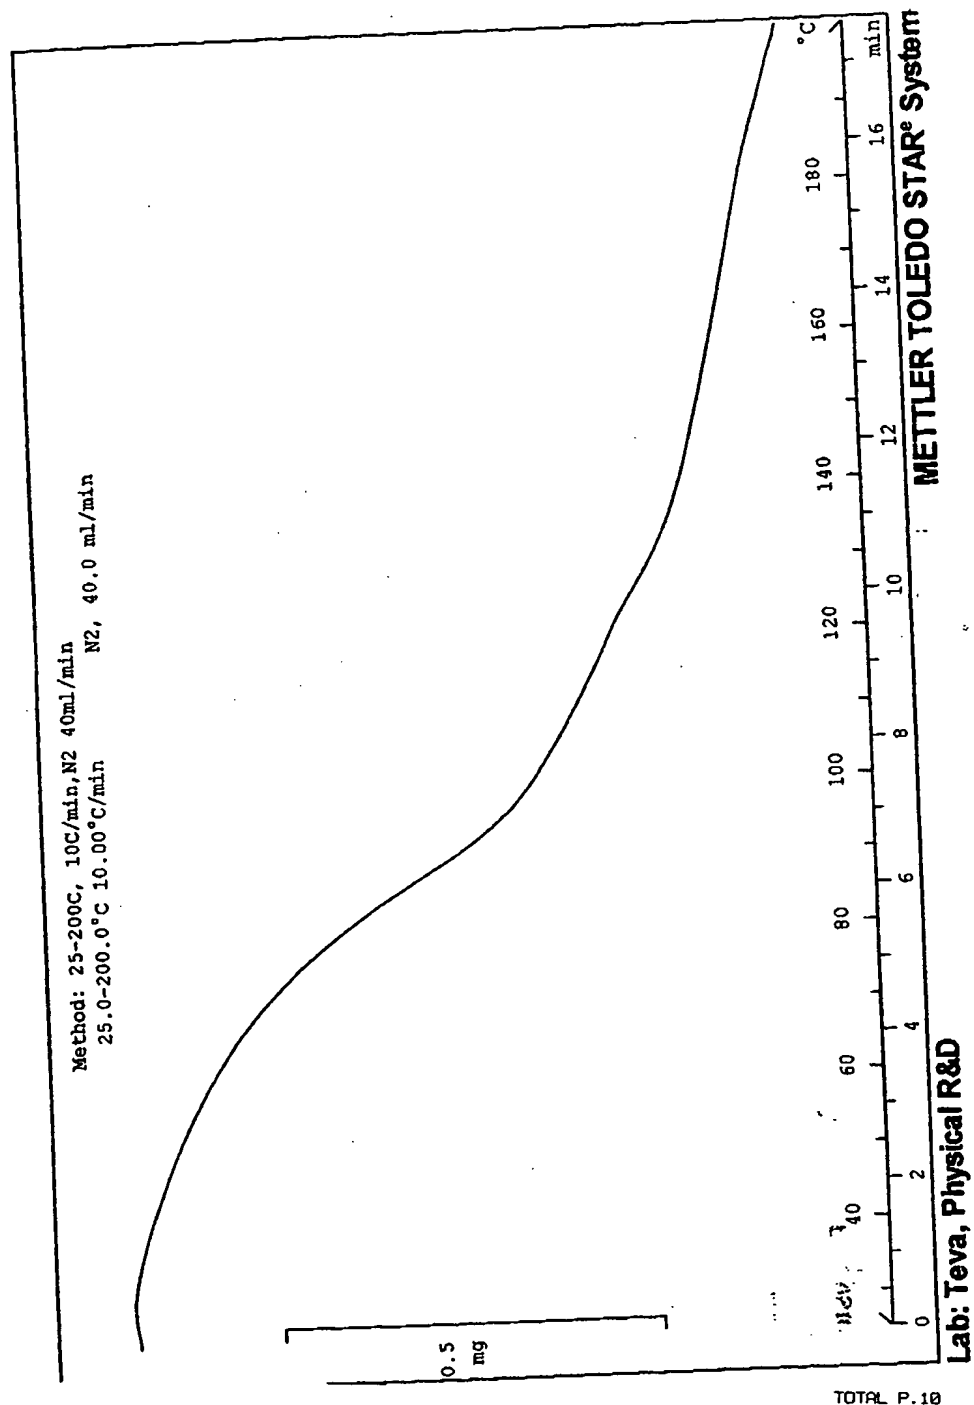


Figure 19


Exo

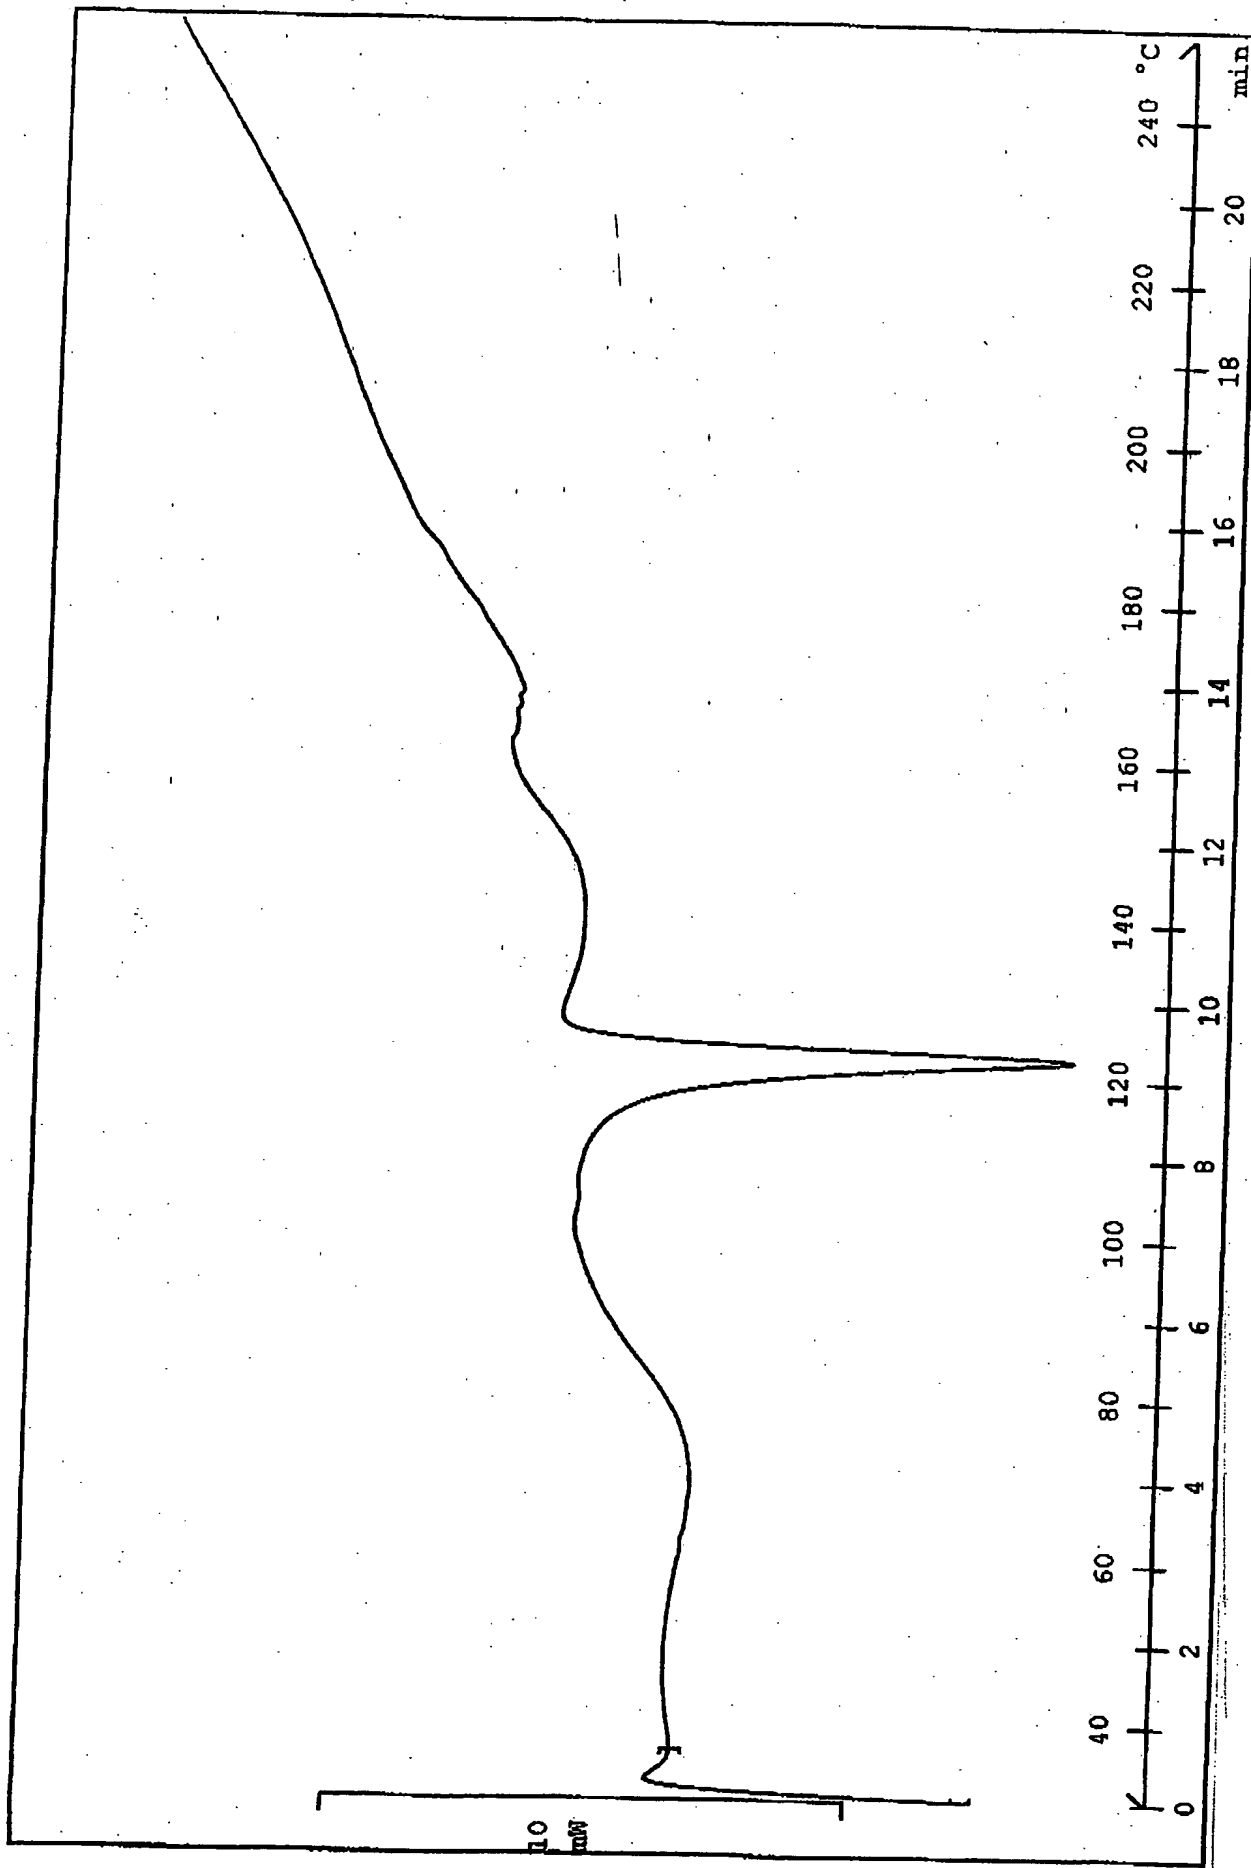

METTLER TOLEDO STAR® System

Figure 20


exo

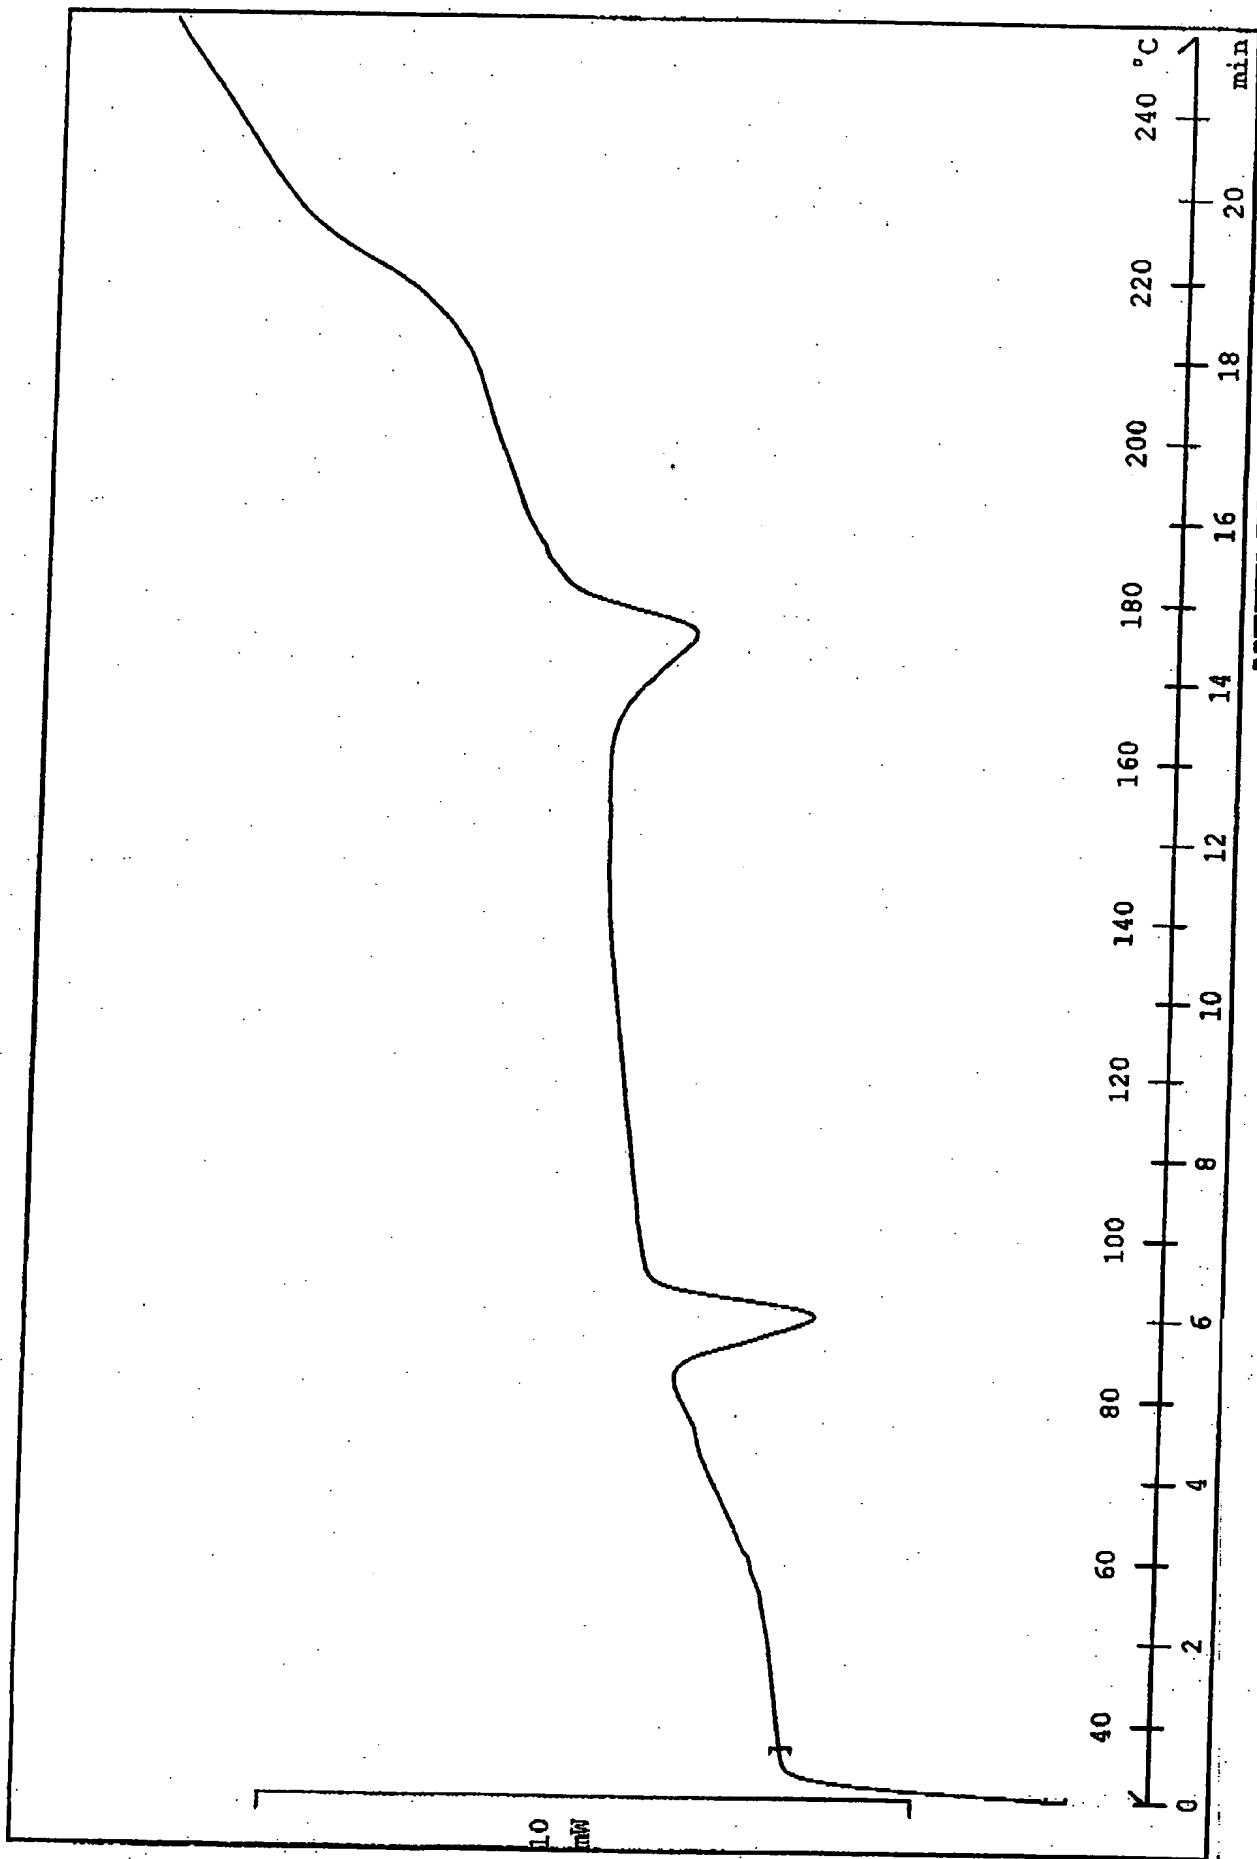

METTLER TOLEDO STAR System

Figure 21

exo

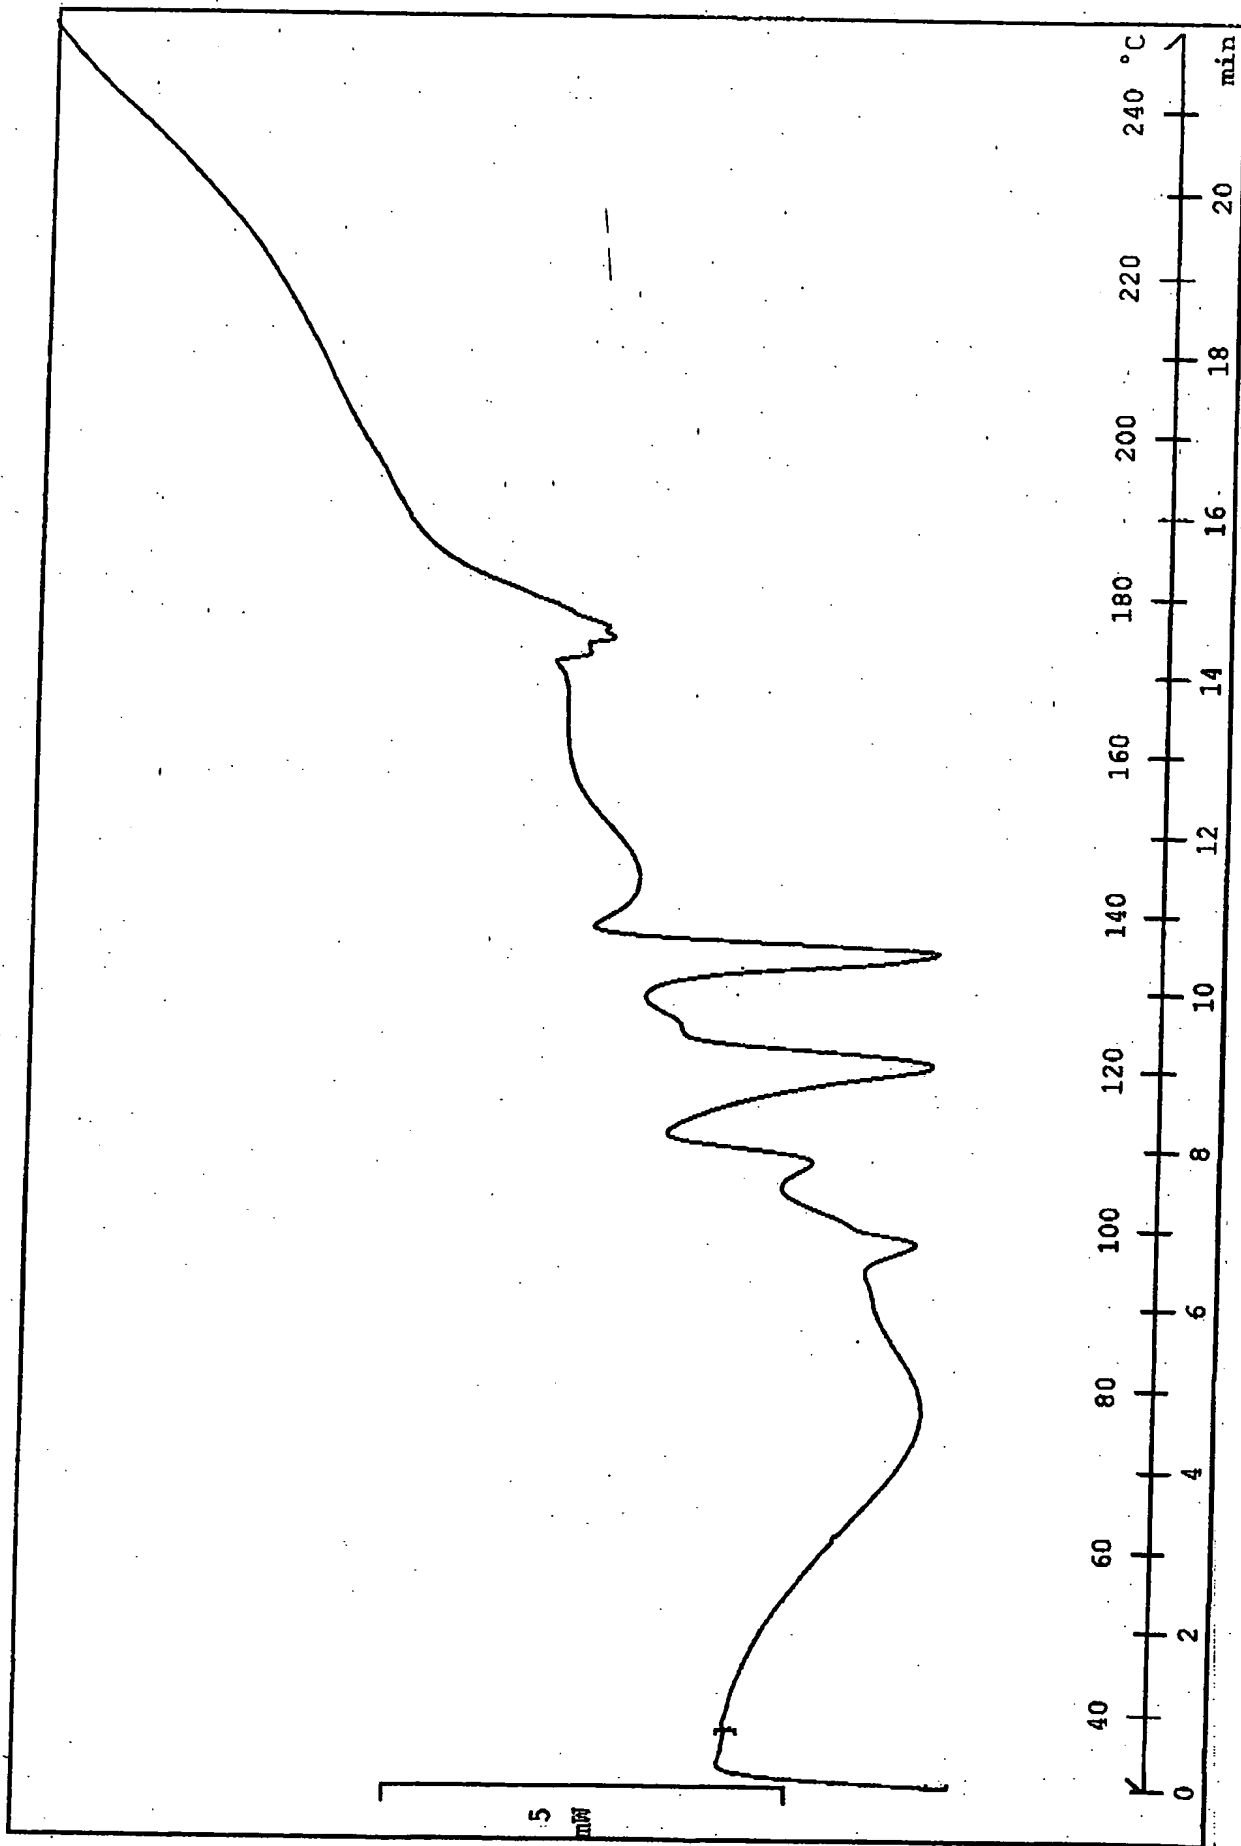

METTTLER TOLEDO STAR® System

Figure 22

Gatifloxacin

3.5210 mg

Method: 30-250°C, 10°C/min, 40ml/min N₂

30.0-250.0°C 10.00°C/min

N₂, 40.0 ml/min

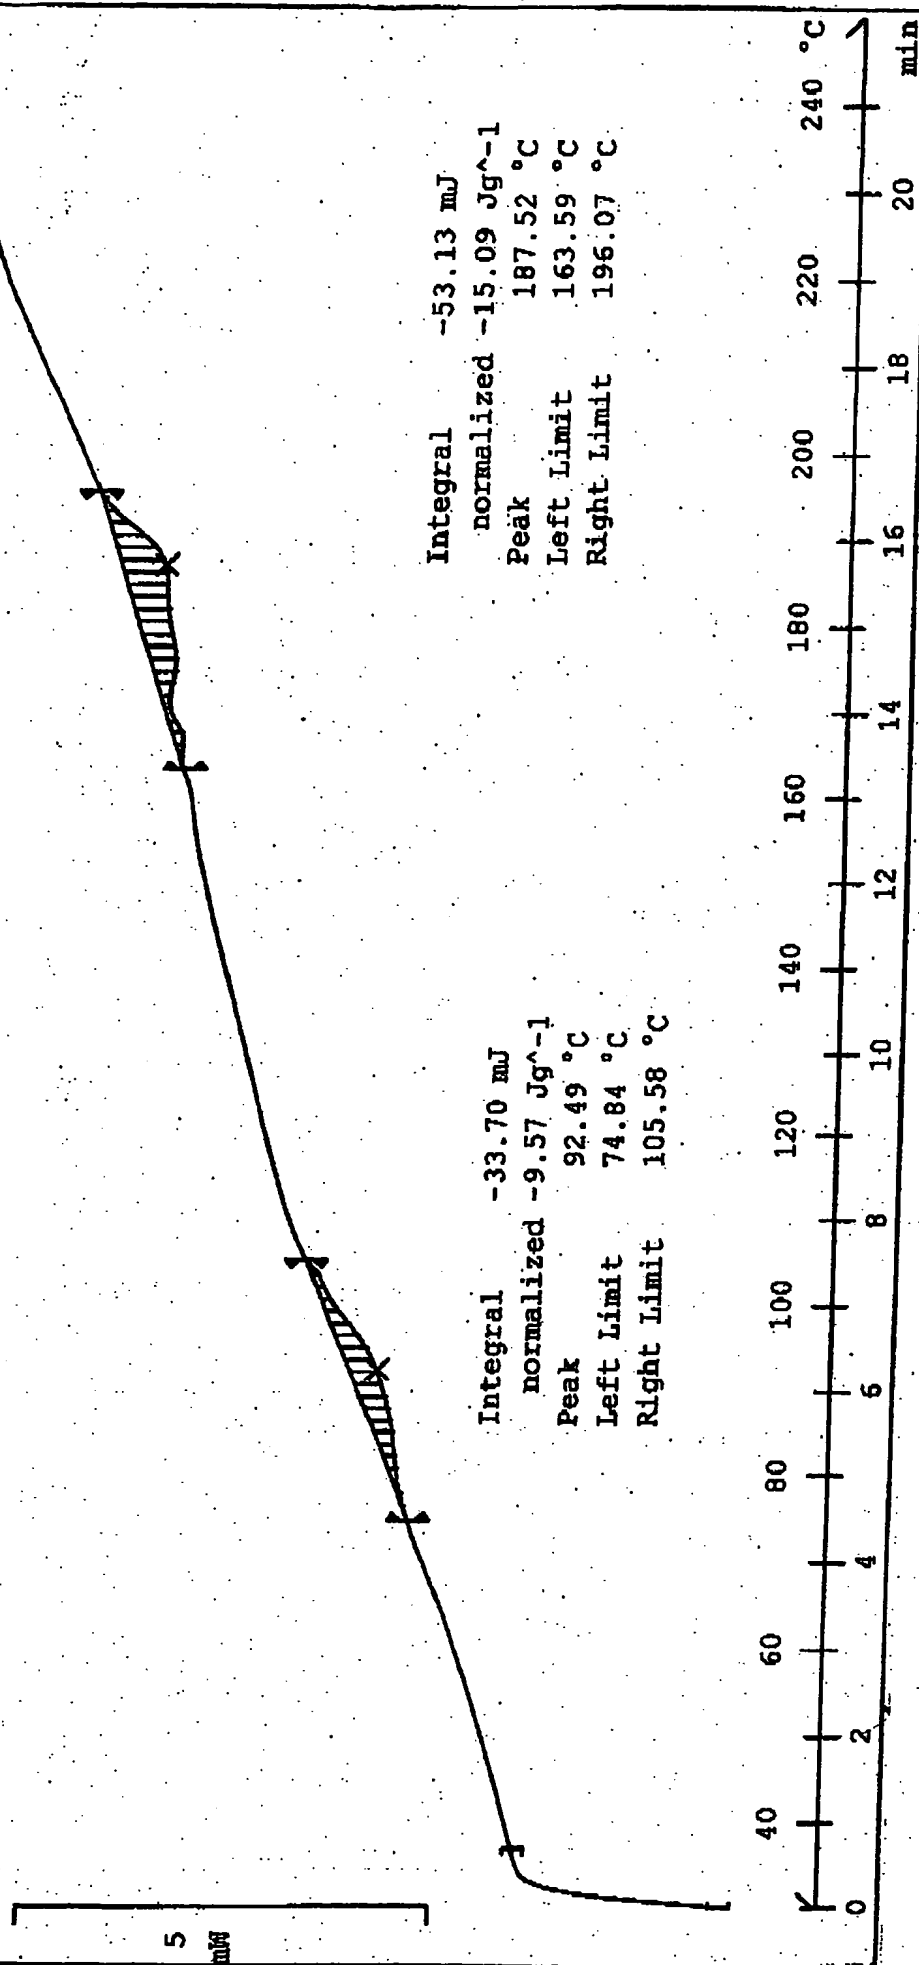


Figure 23

Gatifloxacin

4.2000 mg

Method: 30-250°C, 10°C/min, 40ml/min N2

30.0-250.0°C 10.00°C/min

N2, 40.0 ml/min

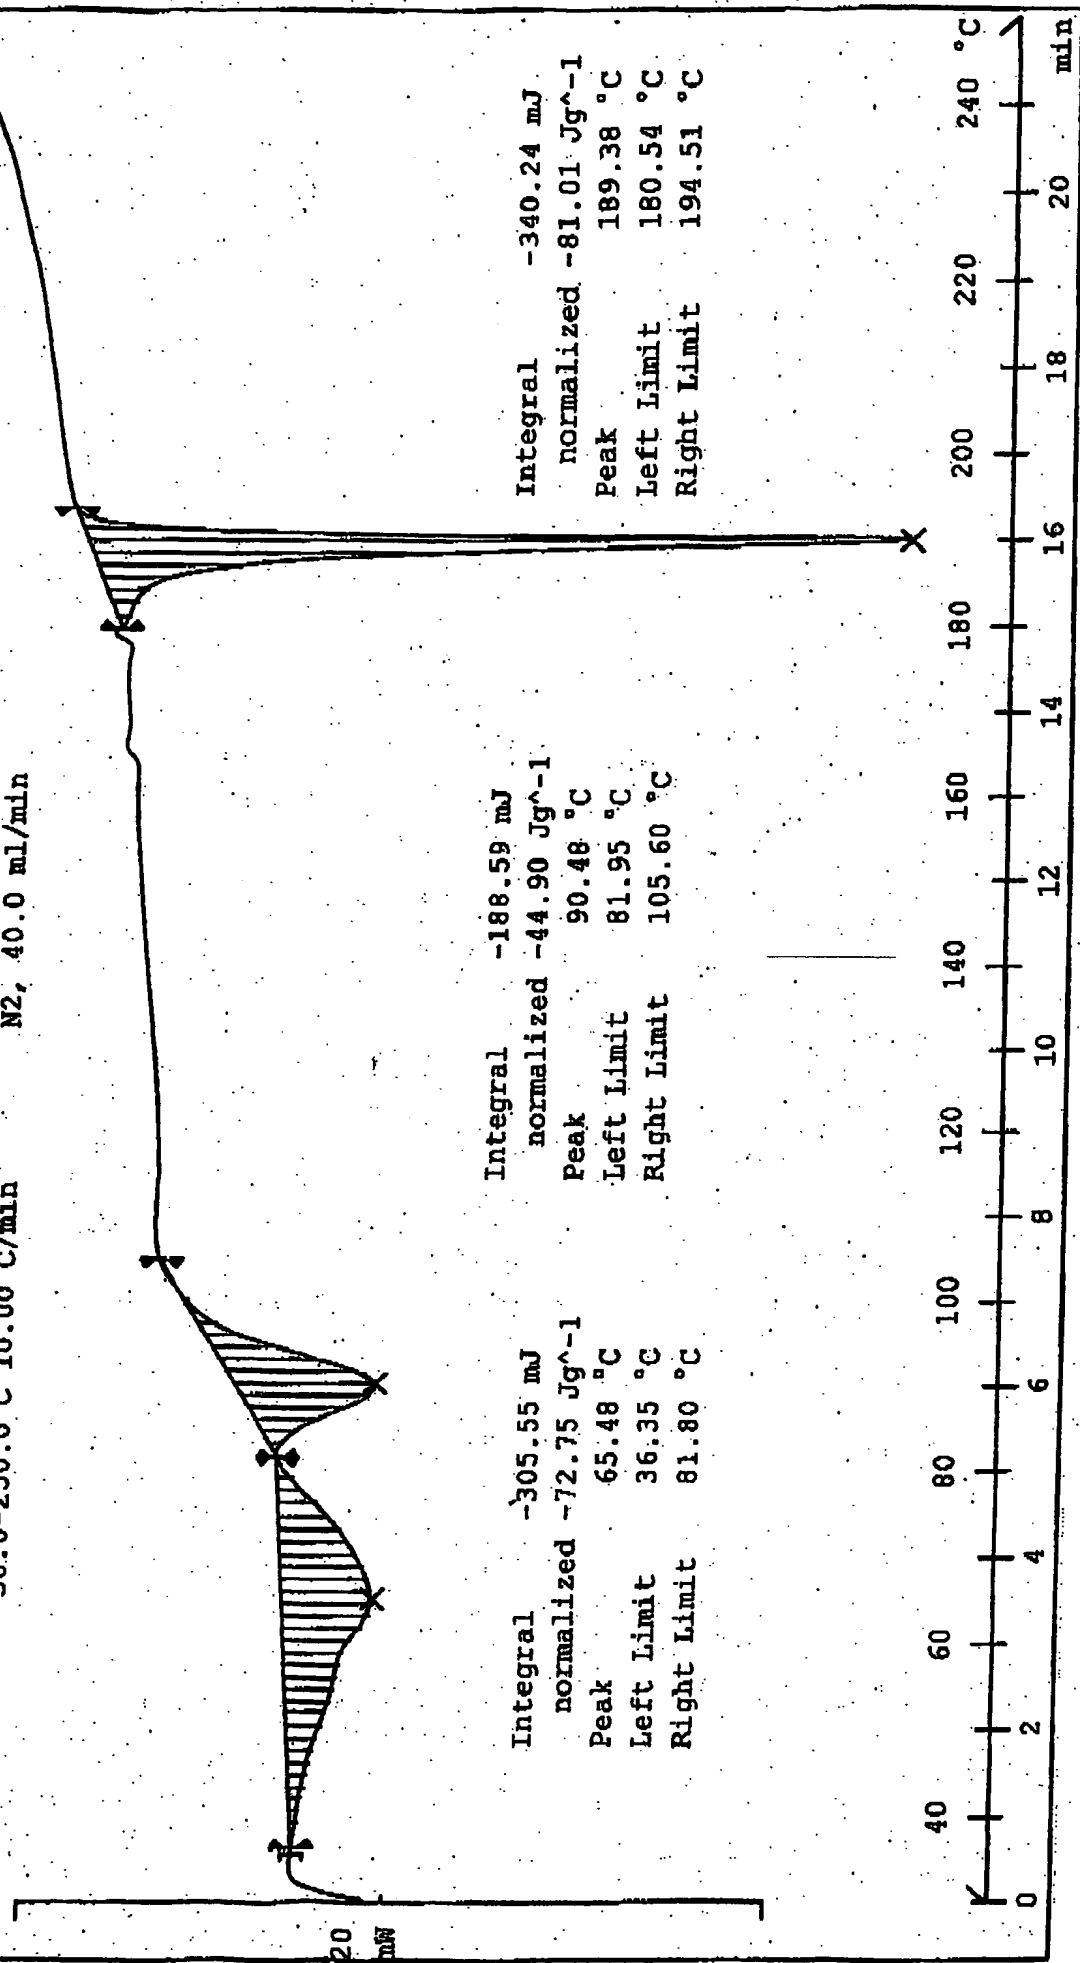


Figure 24

Gatifloxacin
Gatifloxacin

-blank
6.1947 mg

Method: 25-200°C, 10°C/min, N2 40 ml/min
25.0-200.0°C 10.00°C/min N2 40.0 ml/min

0.2
mg

Step -2.192 %
Left Limit -0.180 mg
Right Limit 25.00 °C
Right Limit 120.10 °C

blank corrected curve file: 24.03.03; 09:50:35

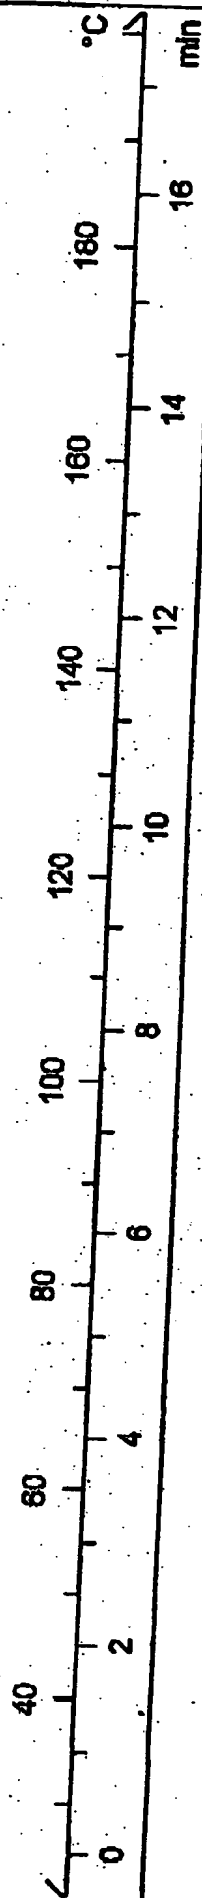


Figure 25

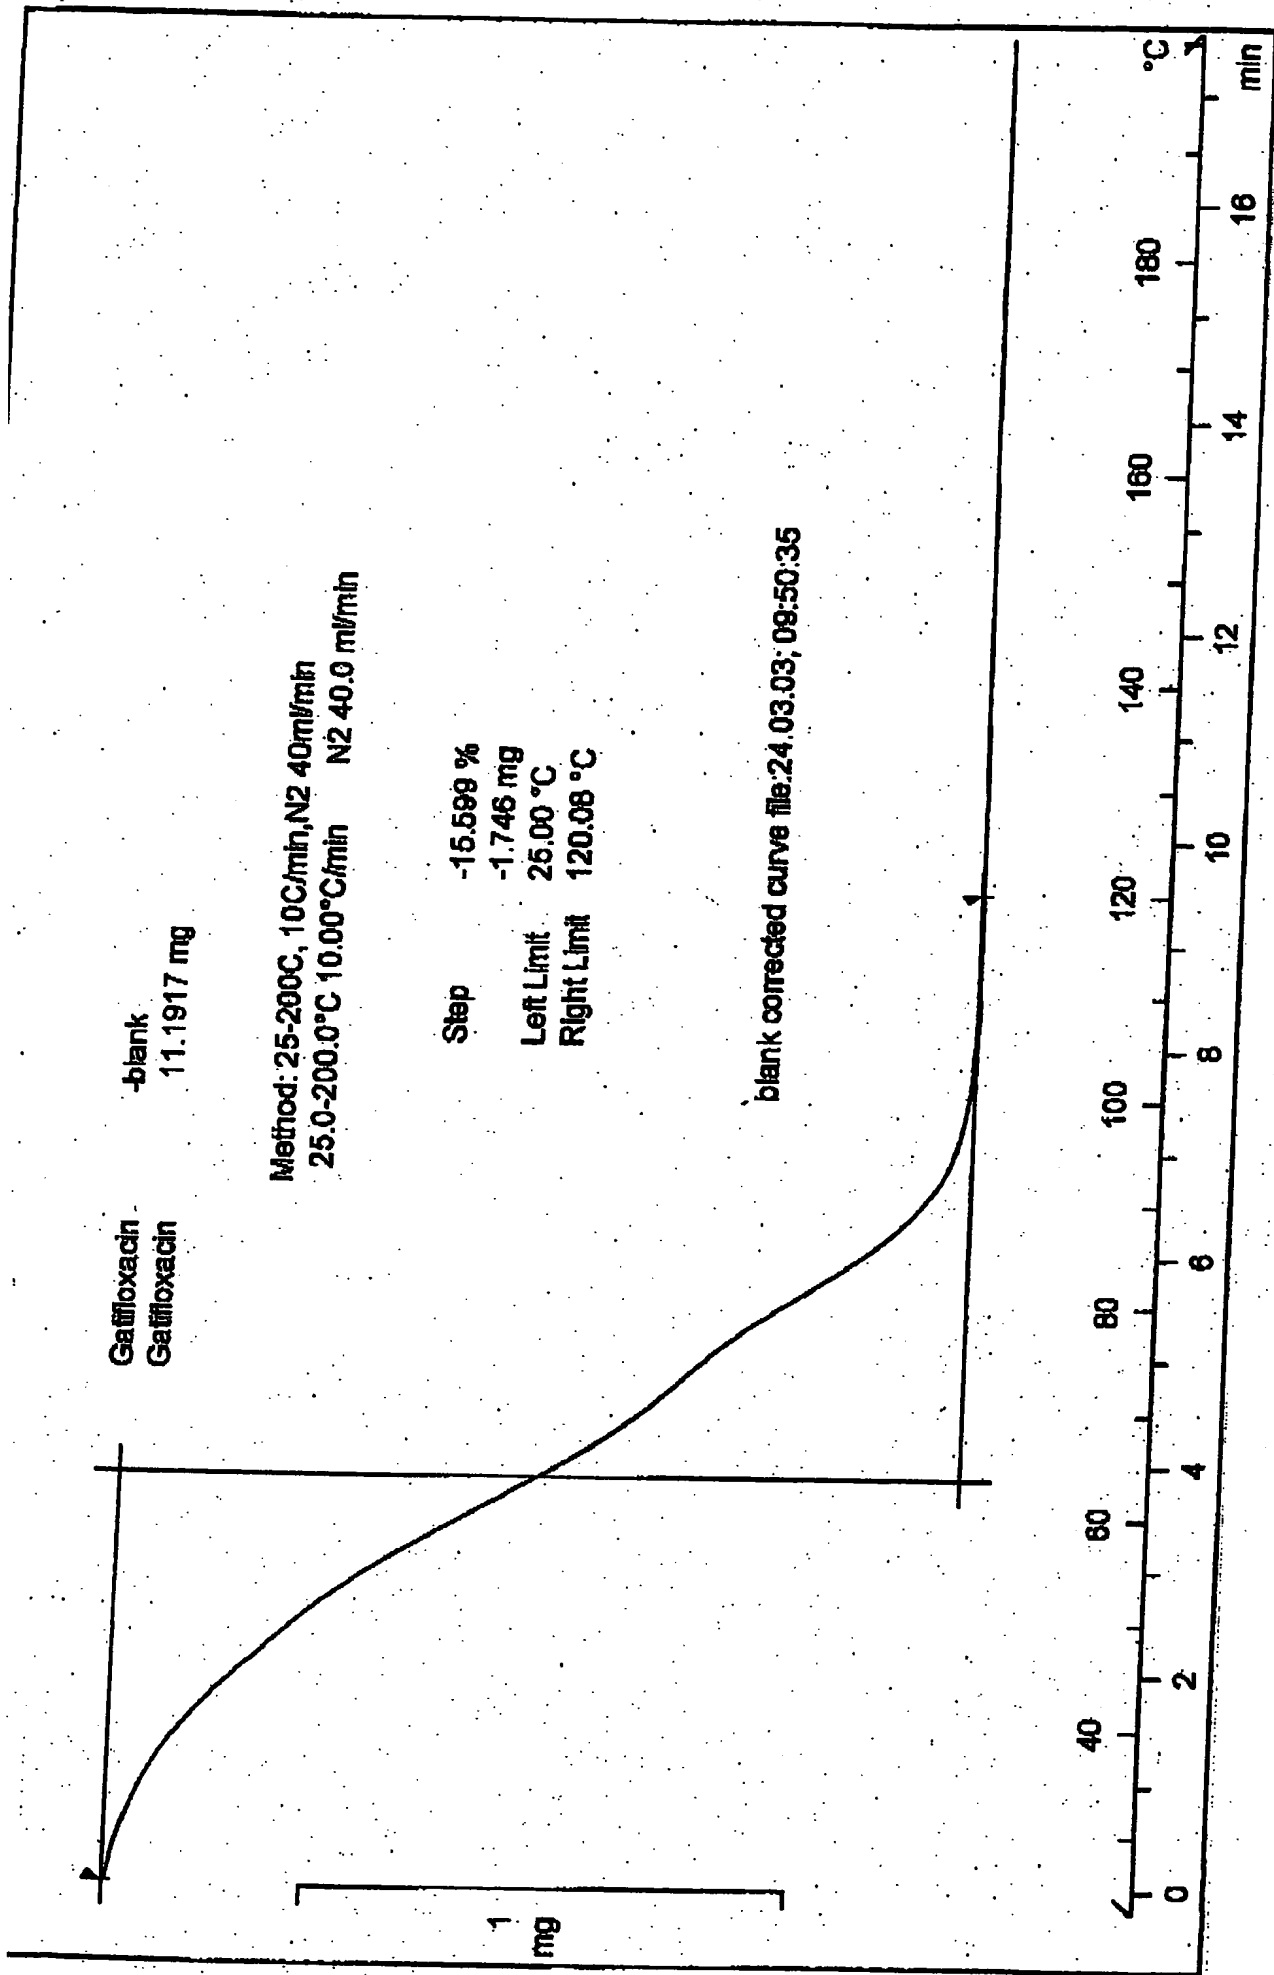


Figure 26